

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
 Data File : VU054747.D
 Acq On : 03 Jul 2023 14:25
 Operator : MD/SY
 Sample : 03495-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	16	21	43	rVB3	29610	48069	4.51%	0.545%
2	1.518	66	71	82	rVB	37830	43466	4.08%	0.493%
3	1.595	86	95	108	rBV	106336	140409	13.18%	1.592%
4	1.907	184	192	211	rVB	86743	133051	12.49%	1.509%
5	2.560	383	395	412	rVB	158369	259778	24.38%	2.946%
6	4.627	1026	1038	1072	rBV2	165048	512342	48.08%	5.811%
7	5.058	1153	1172	1194	rBV	168604	387479	36.36%	4.395%
8	5.721	1356	1378	1407	rBV2	315920	844342	79.24%	9.576%
9	6.245	1524	1541	1565	rBV	315814	615061	57.72%	6.976%
10	6.541	1617	1633	1651	rBV	126742	243612	22.86%	2.763%
11	6.685	1665	1678	1698	rBV	212139	422091	39.61%	4.787%
12	7.563	1939	1951	1971	rBV	102875	182134	17.09%	2.066%
13	7.894	2042	2054	2069	rBV	359697	635542	59.64%	7.208%
14	7.968	2070	2077	2097	rVB	25980	48626	4.56%	0.552%
15	8.177	2128	2142	2156	rBV	64359	112505	10.56%	1.276%
16	8.550	2243	2258	2272	rBV	389591	665644	62.47%	7.550%
17	8.630	2272	2283	2314	rVB2	565790	1065600	100.00%	12.086%
18	8.788	2324	2332	2346	rVB8	8886	17315	1.62%	0.196%
19	9.415	2514	2527	2558	rBV	447052	752749	70.64%	8.537%
20	9.692	2602	2613	2627	rBV2	18664	32507	3.05%	0.369%
21	10.100	2730	2740	2756	rBV5	9225	17368	1.63%	0.197%
22	10.753	2932	2943	2958	rBV	172227	279399	26.22%	3.169%
23	10.891	2973	2986	2996	rBV4	7741	13948	1.31%	0.158%
24	11.466	3156	3165	3175	rBV	9248	14735	1.38%	0.167%
25	11.807	3259	3271	3289	rBV	418190	682951	64.09%	7.746%
26	12.190	3377	3390	3412	rBV	362301	598395	56.16%	6.787%
27	12.884	3598	3606	3619	rBV5	15244	24548	2.30%	0.278%
28	13.209	3695	3707	3718	rBV7	13548	23330	2.19%	0.265%




Sum of corrected areas: 8816996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054747.D
Acq On : 03 Jul 2023 14:25
Operator : MD/SY
Sample : 03495-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

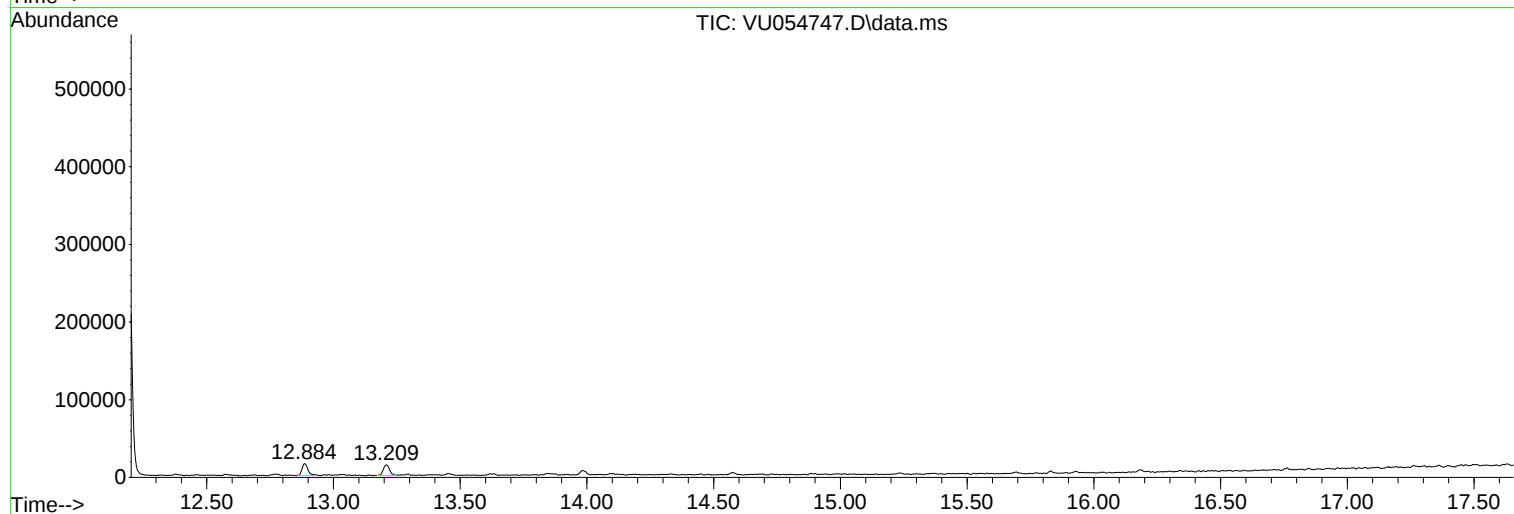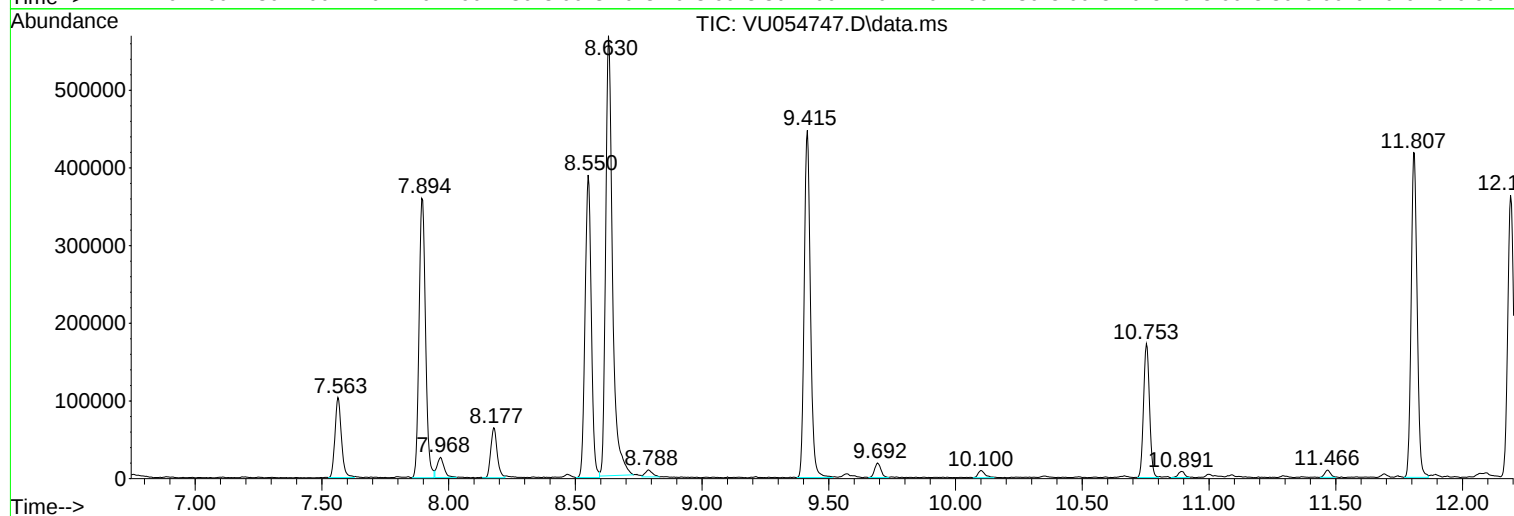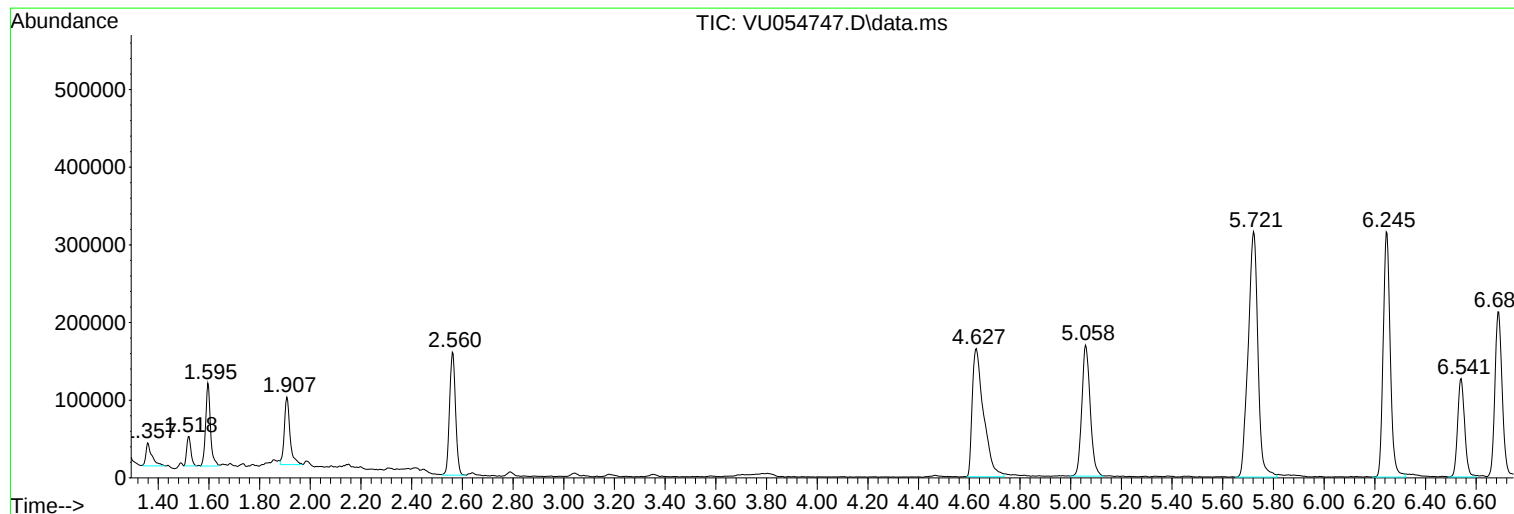

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054747.D
Acq On : 03 Jul 2023 14:25
Operator : MD/SY
Sample : 03495-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070323\
Data File : VU054747.D
Acq On : 03 Jul 2023 14:25
Operator : MD/SY
Sample : 03495-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------