




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059783.D
 Acq On : 03 Jul 2024 09:28
 Operator : MD/SY
 Sample : P3060-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP0

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 06:10:28 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

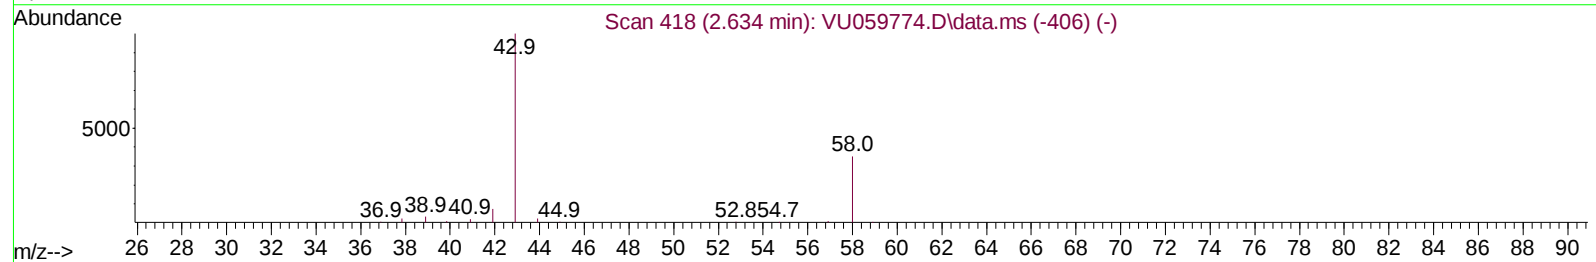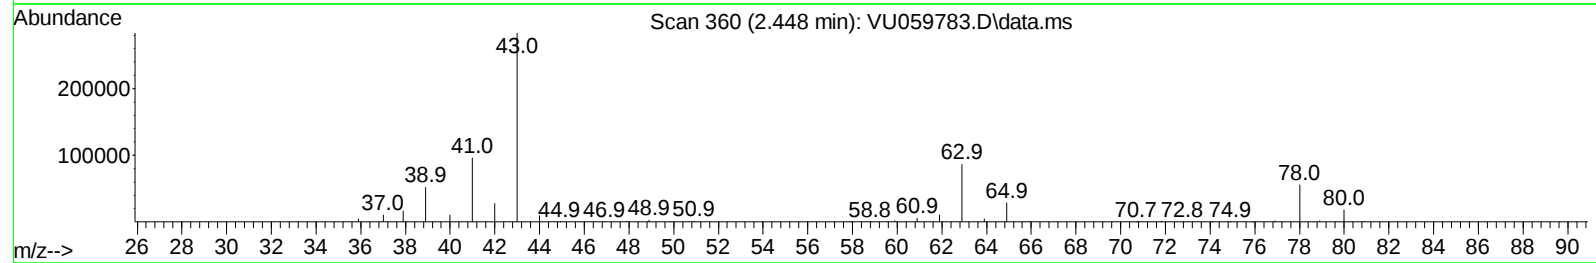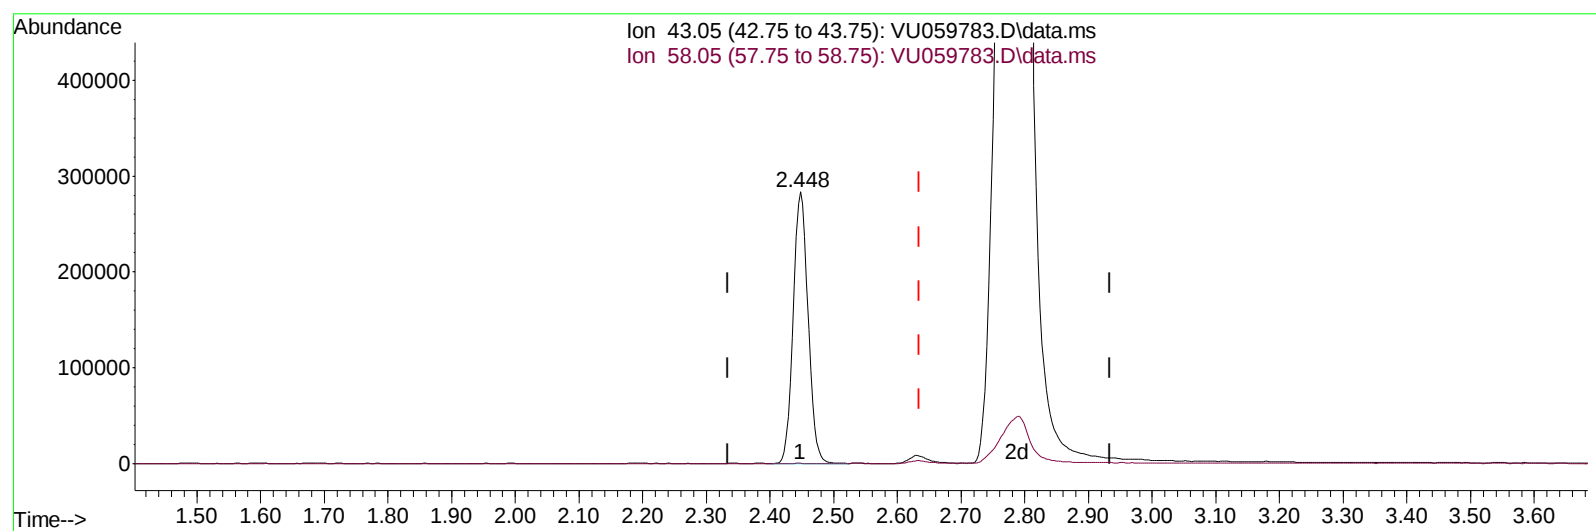

TIC: VU059783.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 310.51 ug/L

response 460160

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059783.D
Acq On : 03 Jul 2024 09:28
Operator : MD/SY
Sample : P3060-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP0

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 06:10:28 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

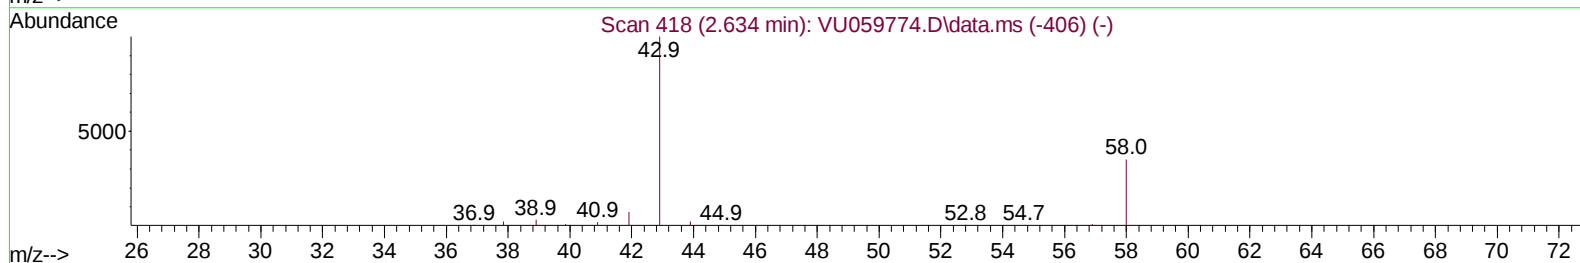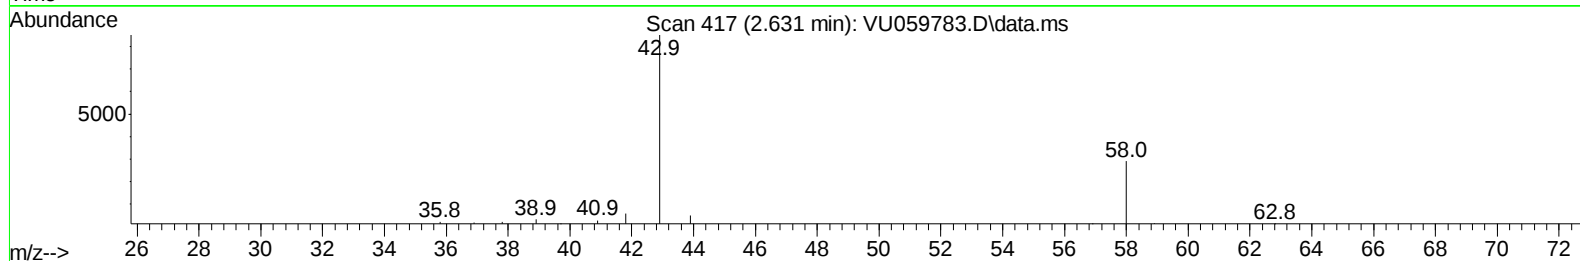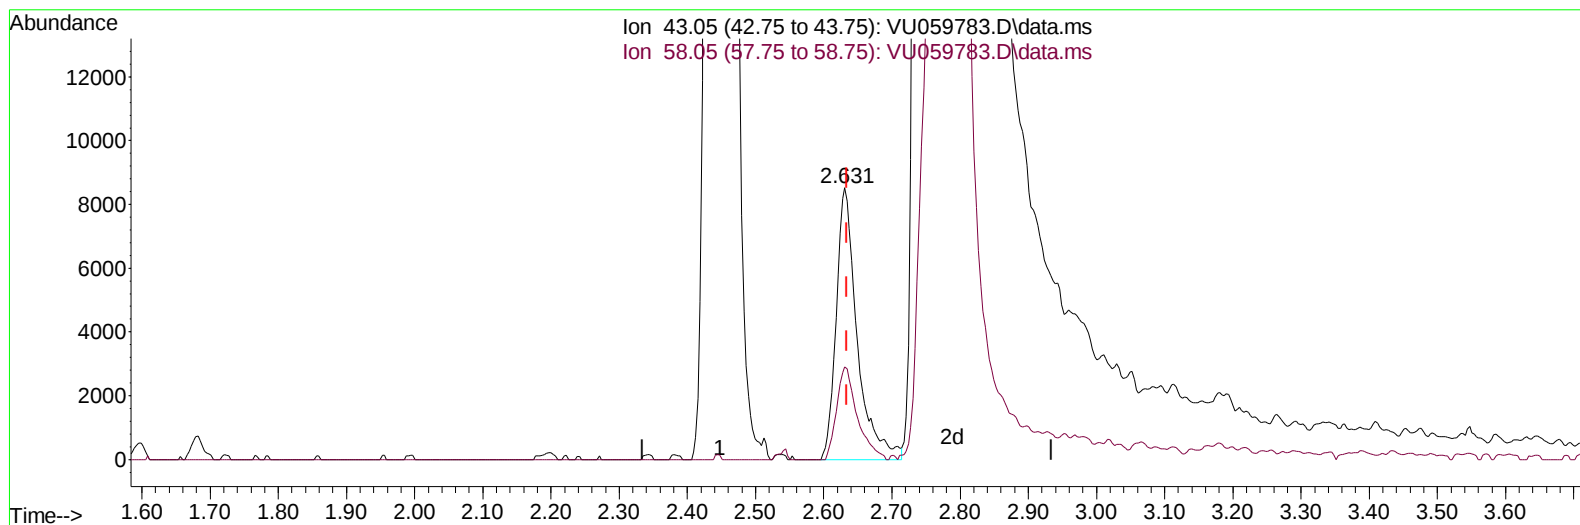

TIC: VU059783.D\data.ms

(13) Acetone (T)

2.631min (-0.003) 12.30 ug/L m

response 18224

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	33.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059783.D
 Acq On : 03 Jul 2024 09:28
 Operator : MD/SY
 Sample : P3060-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP0

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 06:10:28 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		159501	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		165218	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		73284	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		56551	5.099	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.000%	
7) Chloroethane-d5	1.907	69		47179	4.421	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.400%	
11) 1,1-Dichloroethene-d2	2.560	65		20775	4.515	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.400%	
20) 2-Butanone-d5	4.618	46		104154	45.590	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.180%	
24) Chloroform-d	5.052	84		97337	4.276	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%	
26) 1,2-Dichloroethane-d4	5.695	65		48576	4.430	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.600%	
32) Benzene-d6	5.721	84		201028	4.421	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%	
36) 1,2-Dichloropropane-d6	6.682	67		63037	4.524	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.400%	
41) Toluene-d8	7.891	98		172461	4.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.600%	
43) trans-1,3-Dichloroprop...	8.174	79		19394	4.445	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.627	63		81334	44.866	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.740%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		50878	4.419	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.400%	
66) 1,2-Dichlorobenzene-d4	12.187	152		63709	4.884	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.600%	
Target Compounds							
13) Acetone	2.631	43		18224m	12.297	ug/L	
16) Methylene chloride	3.039	84		4126	0.308	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059783.D
Acq On : 03 Jul 2024 09:28
Operator : MD/SY
Sample : P3060-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP0

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 06:10:28 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

