




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059784.D
 Acq On : 03 Jul 2024 09:52
 Operator : MD/SY
 Sample : P3060-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP7

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 06:10:28 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

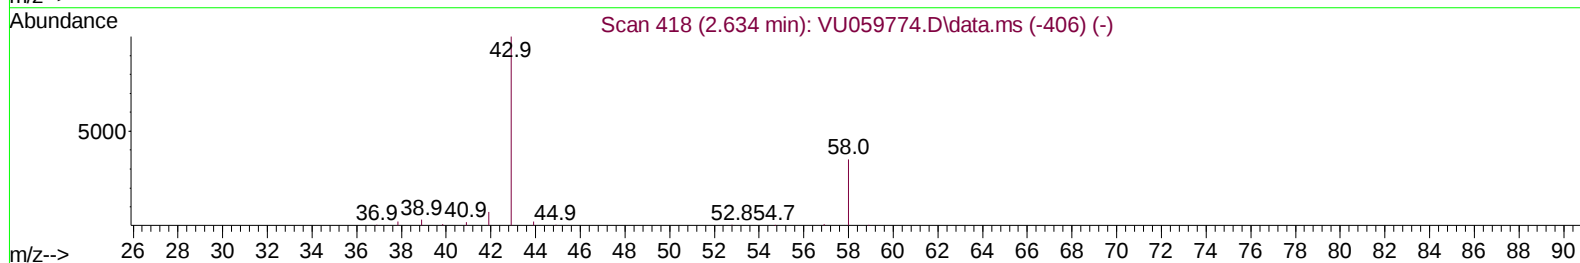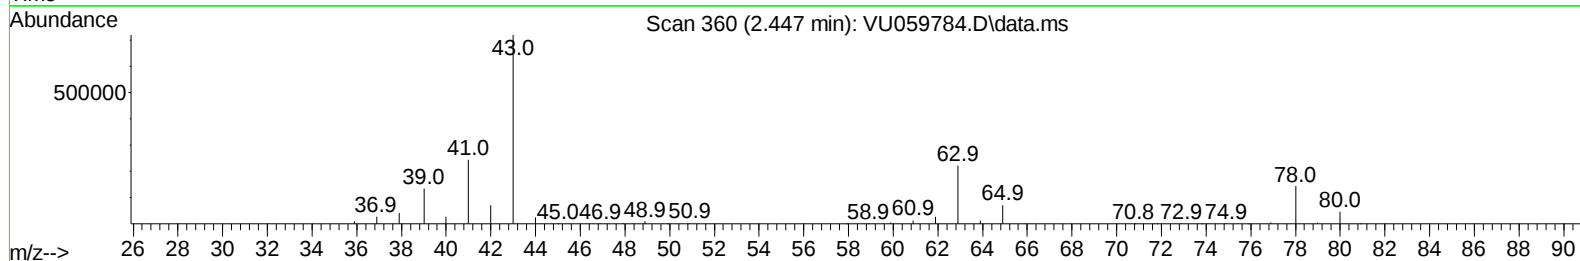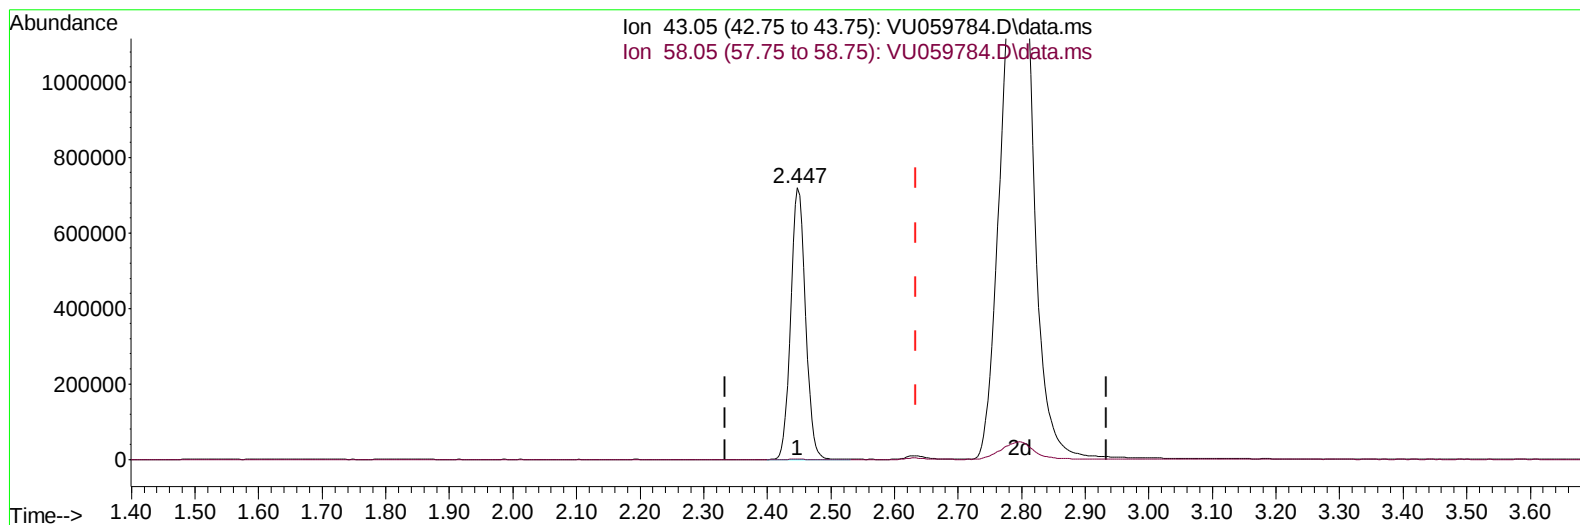

TIC: VU059784.D\data.ms

(13) Acetone (T)

2.447min (-0.187) 763.22 ug/L

response 1165735

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	0.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059784.D
Acq On : 03 Jul 2024 09:52
Operator : MD/SY
Sample : P3060-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP7

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 06:10:28 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

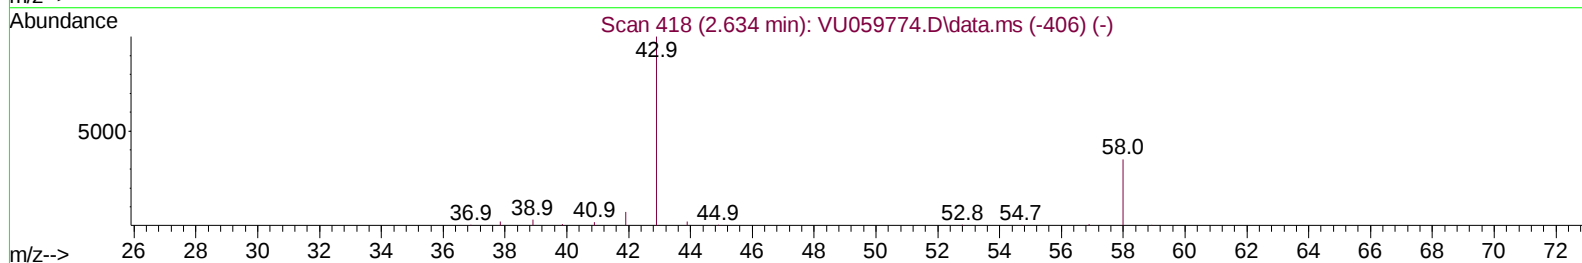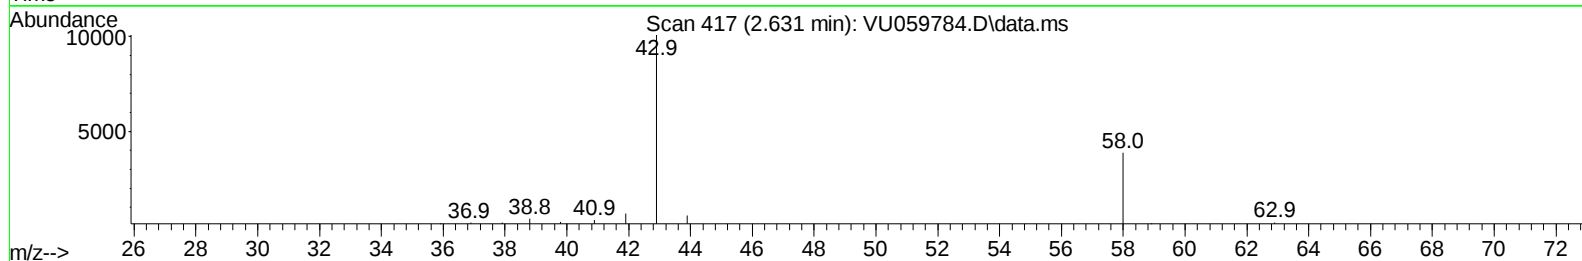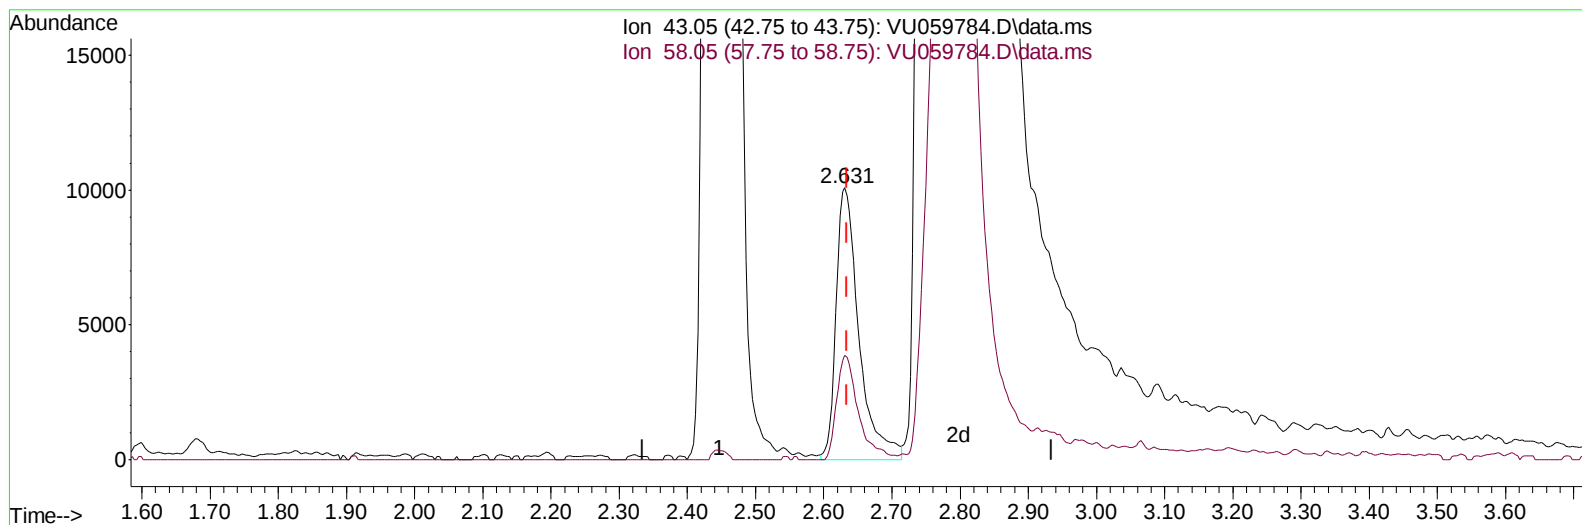

TIC: VU059784.D\data.ms

(13) Acetone (T)

2.631min (-0.003) 15.38 ug/L m

response 23484

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059784.D
 Acq On : 03 Jul 2024 09:52
 Operator : MD/SY
 Sample : P3060-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP7

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 06:10:28 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		164390	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		168460	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		73911	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		56898	4.978	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	99.600%	
7) Chloroethane-d5	1.907	69		48256	4.387	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	87.800%	
11) 1,1-Dichloroethene-d2	2.560	65		21286	4.488	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	89.800%	
20) 2-Butanone-d5	4.618	46		107733	45.754	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	91.500%	
24) Chloroform-d	5.055	84		101199	4.313	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	86.200%	
26) 1,2-Dichloroethane-d4	5.695	65		49846	4.410	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	88.200%	
32) Benzene-d6	5.721	84		205741	4.438	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.800%	
36) 1,2-Dichloropropane-d6	6.682	67		66193	4.659	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	93.200%	
41) Toluene-d8	7.891	98		178781	4.148	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	83.000%	
43) trans-1,3-Dichloroprop...	8.177	79		20100	4.518	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	90.400%	
46) 2-Hexanone-d5	8.627	63		84226	45.567	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	91.140%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		52367	4.461	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	89.200%	
66) 1,2-Dichlorobenzene-d4	12.187	152		65525	4.981	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	99.600%	
Target Compounds							
13) Acetone	2.631	43		23484m	15.375	ug/L	
16) Methylene chloride	3.039	84		3809	0.276	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059784.D
Acq On : 03 Jul 2024 09:52
Operator : MD/SY
Sample : P3060-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP7

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 06:10:28 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

