




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059785.D
 Acq On : 03 Jul 2024 10:16
 Operator : MD/SY
 Sample : P3060-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP8

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 06:10:28 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

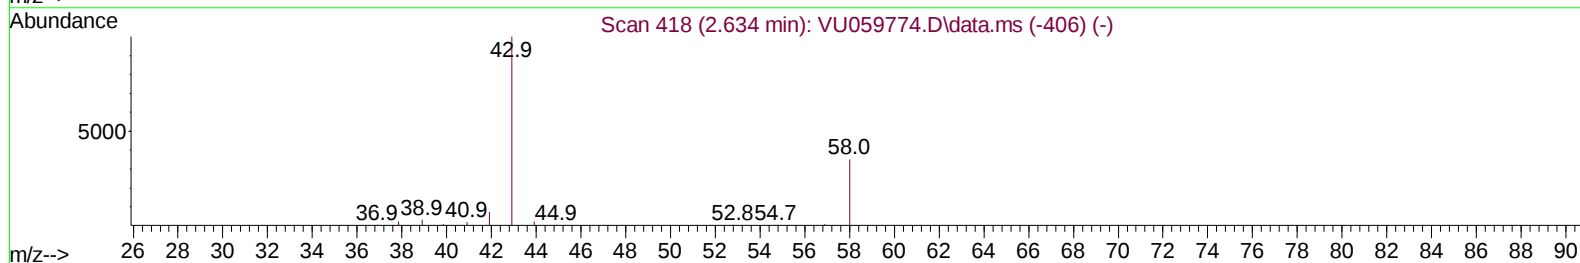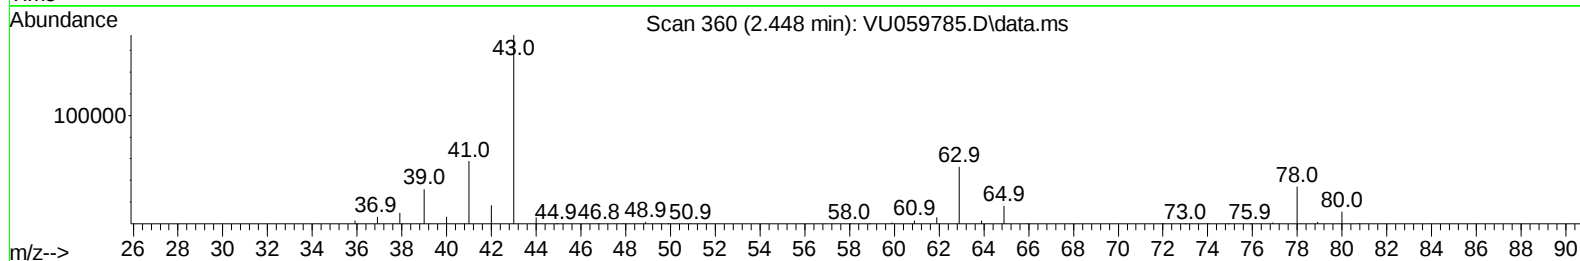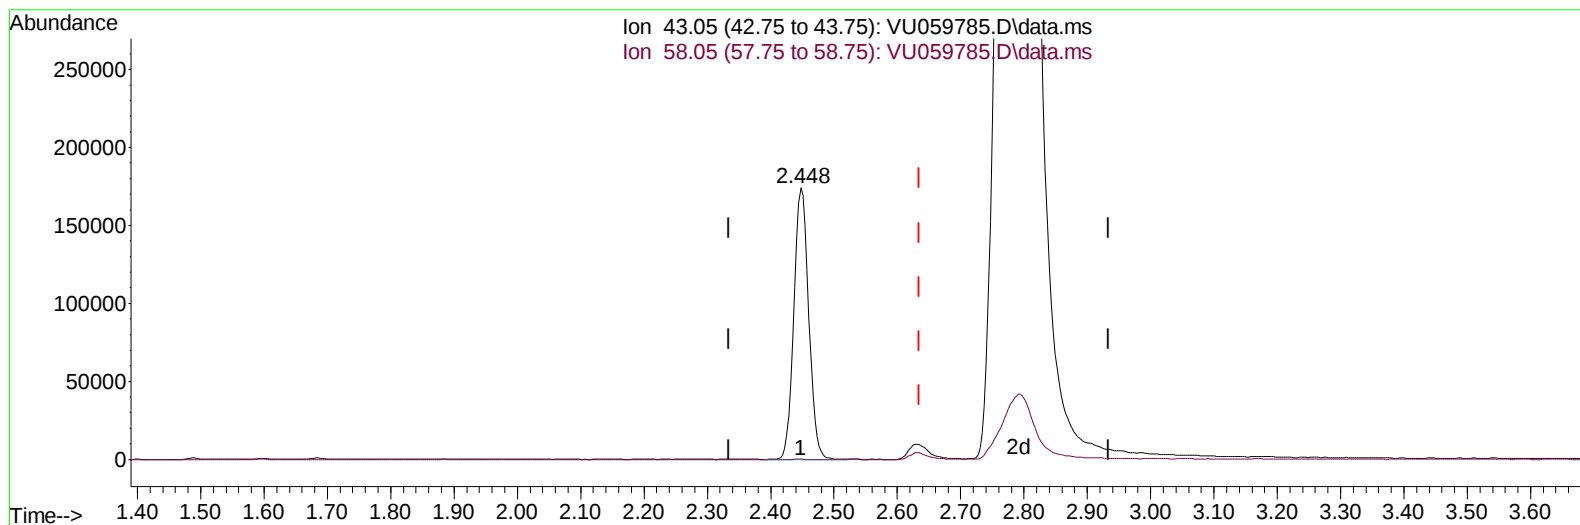

TIC: VU059785.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 187.46 ug/L

response 283362

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	3.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059785.D
Acq On : 03 Jul 2024 10:16
Operator : MD/SY
Sample : P3060-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP8

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 06:10:28 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

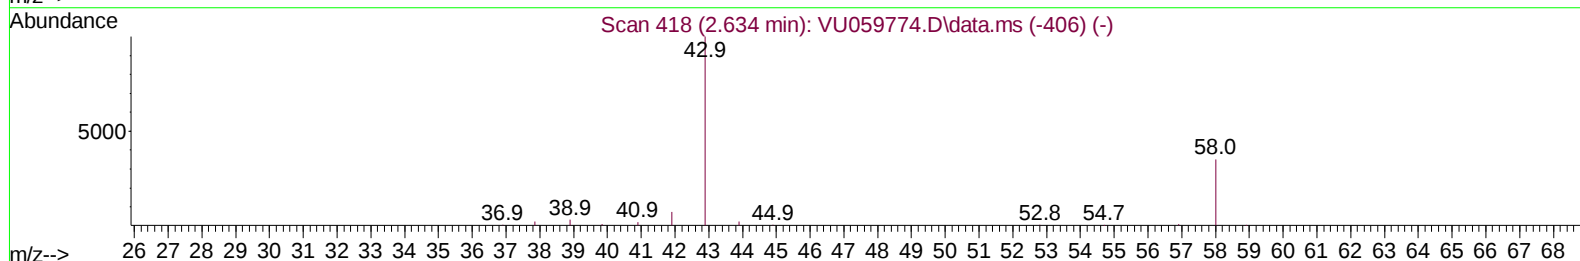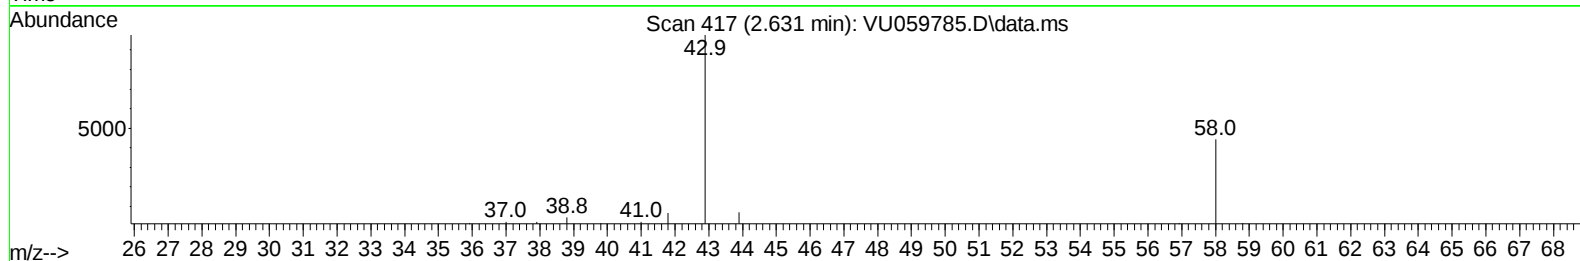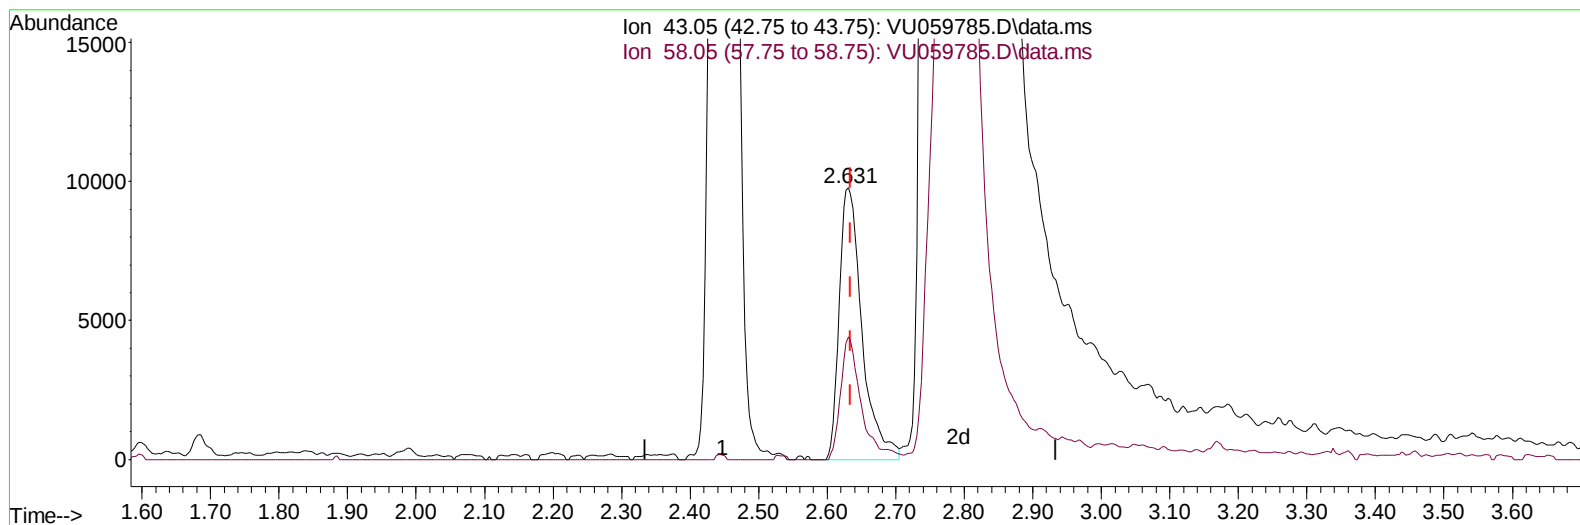

TIC: VU059785.D\data.ms

(13) Acetone (T)

2.631min (-0.003) 14.91 ug/L m

response 22530

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	41.14
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059785.D
 Acq On : 03 Jul 2024 10:16
 Operator : MD/SY
 Sample : P3060-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP8

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 06:10:28 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		162687	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		166010	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		72255	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		53430	4.723	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	94.400%	
7) Chloroethane-d5	1.907	69		45001	4.134	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	82.600%	
11) 1,1-Dichloroethene-d2	2.560	65		19097	4.069	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	81.400%	
20) 2-Butanone-d5	4.618	46		99819	42.837	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	85.680%	
24) Chloroform-d	5.055	84		94126	4.054	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	81.000%	
26) 1,2-Dichloroethane-d4	5.695	65		46555	4.162	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	83.200%	
32) Benzene-d6	5.721	84		190105	4.161	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	83.200%	
36) 1,2-Dichloropropane-d6	6.682	67		61852	4.418	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	88.400%	
41) Toluene-d8	7.891	98		162164	3.818	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	76.400%	
43) trans-1,3-Dichloroprop...	8.174	79		18486	4.217	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	84.400%	
46) 2-Hexanone-d5	8.627	63		77392	42.488	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	84.980%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		47572	4.113	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	82.200%	
66) 1,2-Dichlorobenzene-d4	12.187	152		60248	4.685	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	93.600%	
Target Compounds							
13) Acetone	2.631	43		22530m	14.905	ug/L	
16) Methylene chloride	3.036	84		4649	0.340	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059785.D
Acq On : 03 Jul 2024 10:16
Operator : MD/SY
Sample : P3060-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP8

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:56:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 06:10:28 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

