




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059836.D
Acq On : 04 Jul 2024 08:16
Operator : MD/SY
Sample : P3109-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0HC1

Manual IntegrationsAPPROVED

Quant Time: Jul 04 09:03:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 04 04:26:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

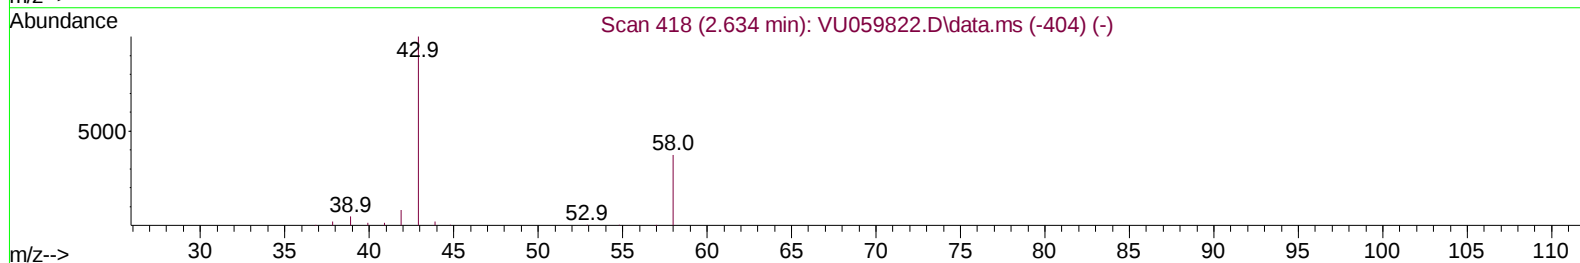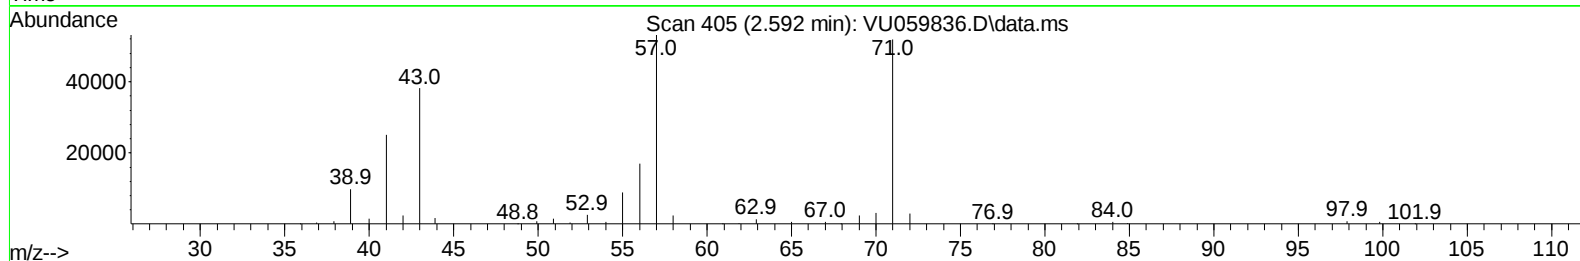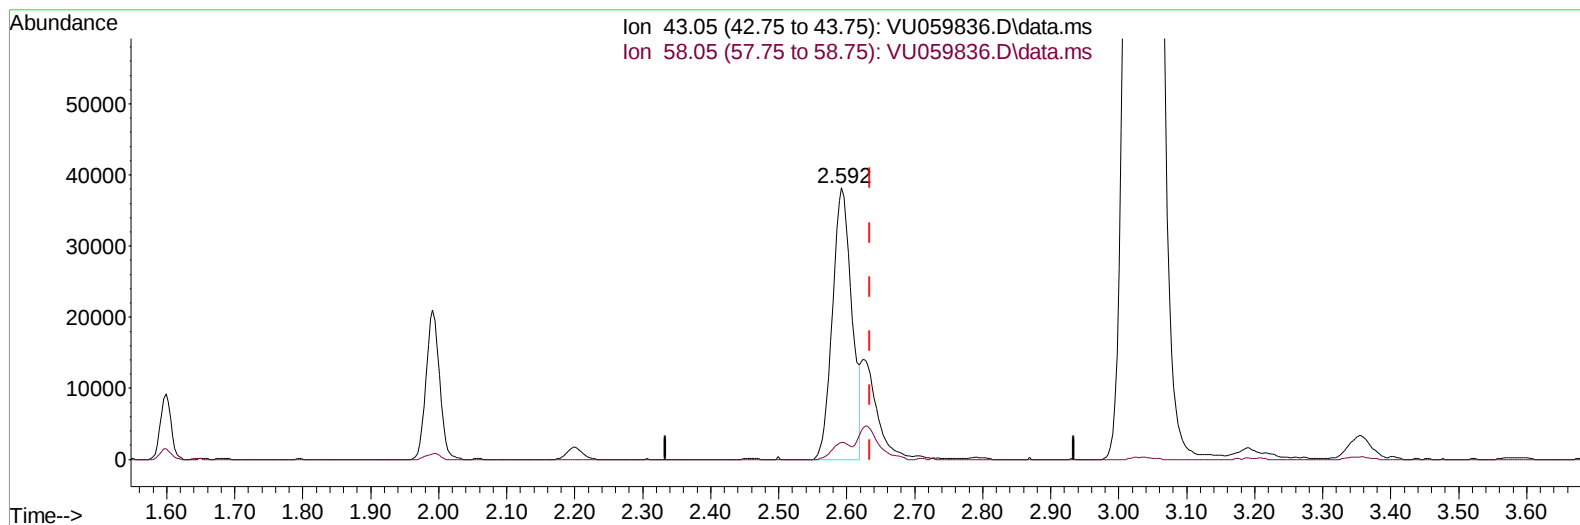

TIC: VU059836.D\data.ms

(13) Acetone (T)

2.592min (-0.042) 48.67 ug/L

response 74867

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	6.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059836.D
Acq On : 04 Jul 2024 08:16
Operator : MD/SY
Sample : P3109-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0HC1

Manual IntegrationsAPPROVED

Quant Time: Jul 04 09:03:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 04 04:26:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

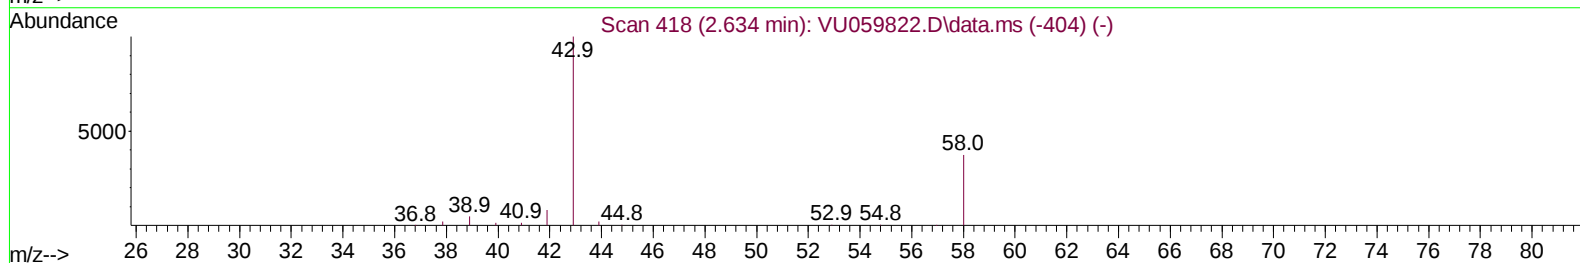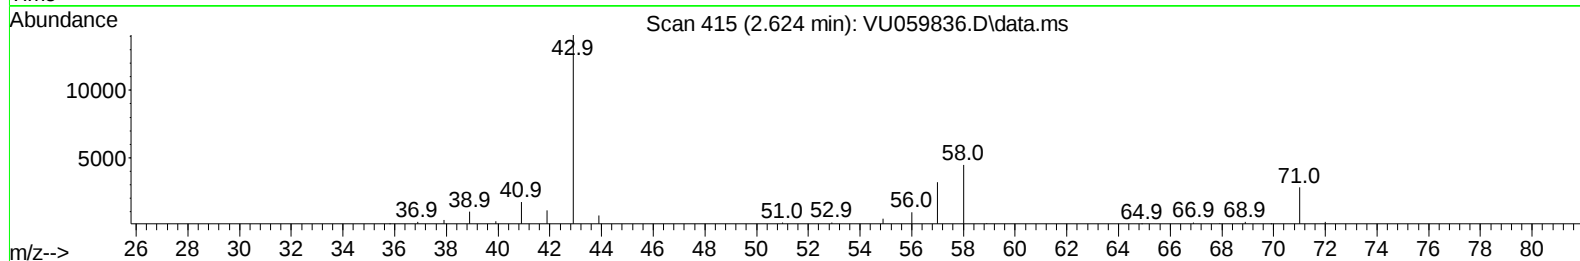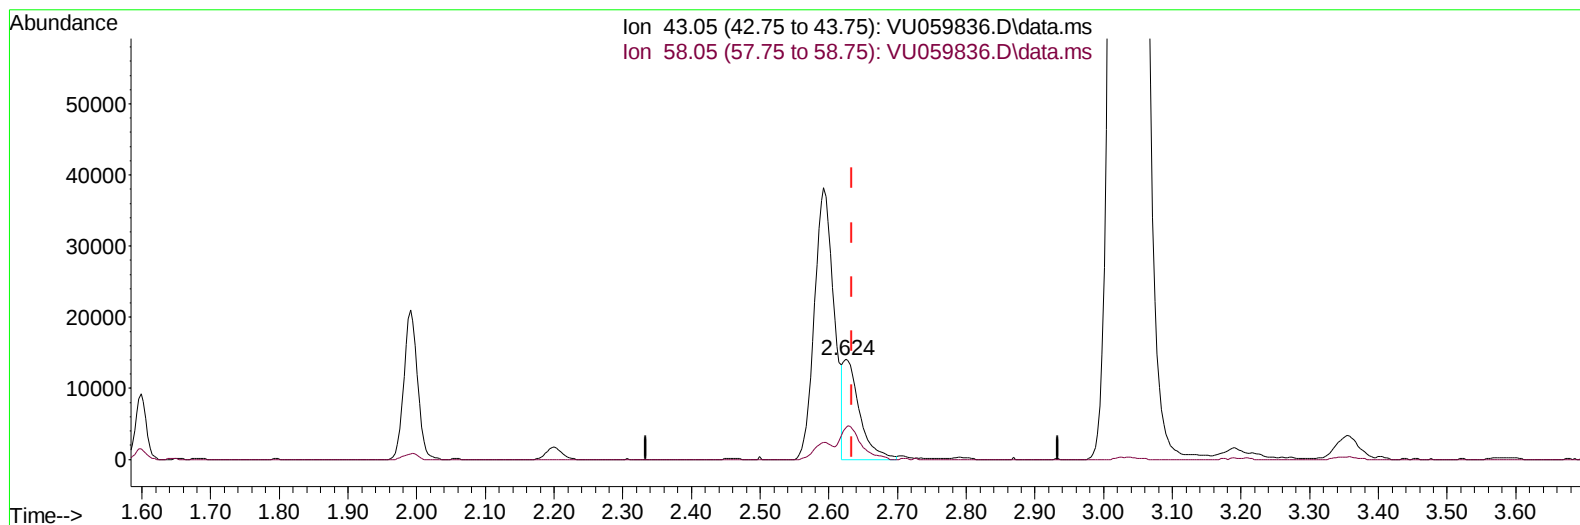

TIC: VU059836.D\data.ms

(13) Acetone (T)

2.624min (-0.010) 15.40 ug/L m

response 23689

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	19.13
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059836.D
 Acq On : 04 Jul 2024 08:16
 Operator : MD/SY
 Sample : P3109-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0HC1

Manual IntegrationsAPPROVED

Quant Time: Jul 04 09:03:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 04 04:26:48 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		165553	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		162883	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		81065	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		50015	4.345	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	86.800%	
7) Chloroethane-d5	1.911	69		45212	4.082	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	81.600%	
11) 1,1-Dichloroethene-d2	2.560	65		20009	4.190	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	83.800%	
20) 2-Butanone-d5	4.618	46		112541	47.460	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	94.920%	
24) Chloroform-d	5.055	84		98767	4.180	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	83.600%	
26) 1,2-Dichloroethane-d4	5.695	65		48918	4.298	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	86.000%	
32) Benzene-d6	5.718	84		207575	4.630	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	6.682	67		69063	5.028	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	100.600%	
41) Toluene-d8	7.891	98		191116	4.586	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	91.800%	
43) trans-1,3-Dichloroprop...	8.174	79		21577	5.016	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	100.400%	
46) 2-Hexanone-d5	8.624	63		100732	56.363	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	112.720%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		52609	4.635	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	92.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		72168	5.002	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	100.000%	
Target Compounds							
13) Acetone	2.624	43		23689m	15.400	ug/L	
17) Methyl tert-butyl Ether	3.358	73		33848	1.338	ug/L #	76
27) 1,2-Dichloroethane	5.785	62		32539	2.264	ug/L #	82
63) 1,2,4-Trimethylbenzene	11.463	105		9544	0.252	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059836.D
Acq On : 04 Jul 2024 08:16
Operator : MD/SY
Sample : P3109-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0HC1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

Quant Time: Jul 04 09:03:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 04 04:26:48 2024
Response via : Initial Calibration

