

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059763.D
 Acq On : 03 Jul 2024 01:33
 Operator : MD/SY
 Sample : P3121-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BK2

Quant Time: Jul 03 04:10:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 04:07:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	163038	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	169223	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	74874	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	54692	4.824	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.400%
7) Chloroethane-d5	1.907	69	46281	4.243	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.800%
11) 1,1-Dichloroethene-d2	2.560	65	20426	4.343	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.800%
20) 2-Butanone-d5	4.624	46	101936	43.651	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.300%
24) Chloroform-d	5.055	84	95652	4.111	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.200%
26) 1,2-Dichloroethane-d4	5.695	65	46837	4.178	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
32) Benzene-d6	5.721	84	196220	4.213	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.200%
36) 1,2-Dichloropropane-d6	6.682	67	62009	4.345	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.000%
41) Toluene-d8	7.891	98	168656	3.895	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
43) trans-1,3-Dichloroprop...	8.177	79	18987	4.249	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.627	63	82065	44.198	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.400%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	49196	4.172	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	61786	4.636	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.800%
Target Compounds					Qvalue	
13) Acetone	2.637	43	8297	5.477	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059763.D
Acq On : 03 Jul 2024 01:33
Operator : MD/SY
Sample : P3121-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BK2

Quant Time: Jul 03 04:10:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 04:07:12 2024
Response via : Initial Calibration

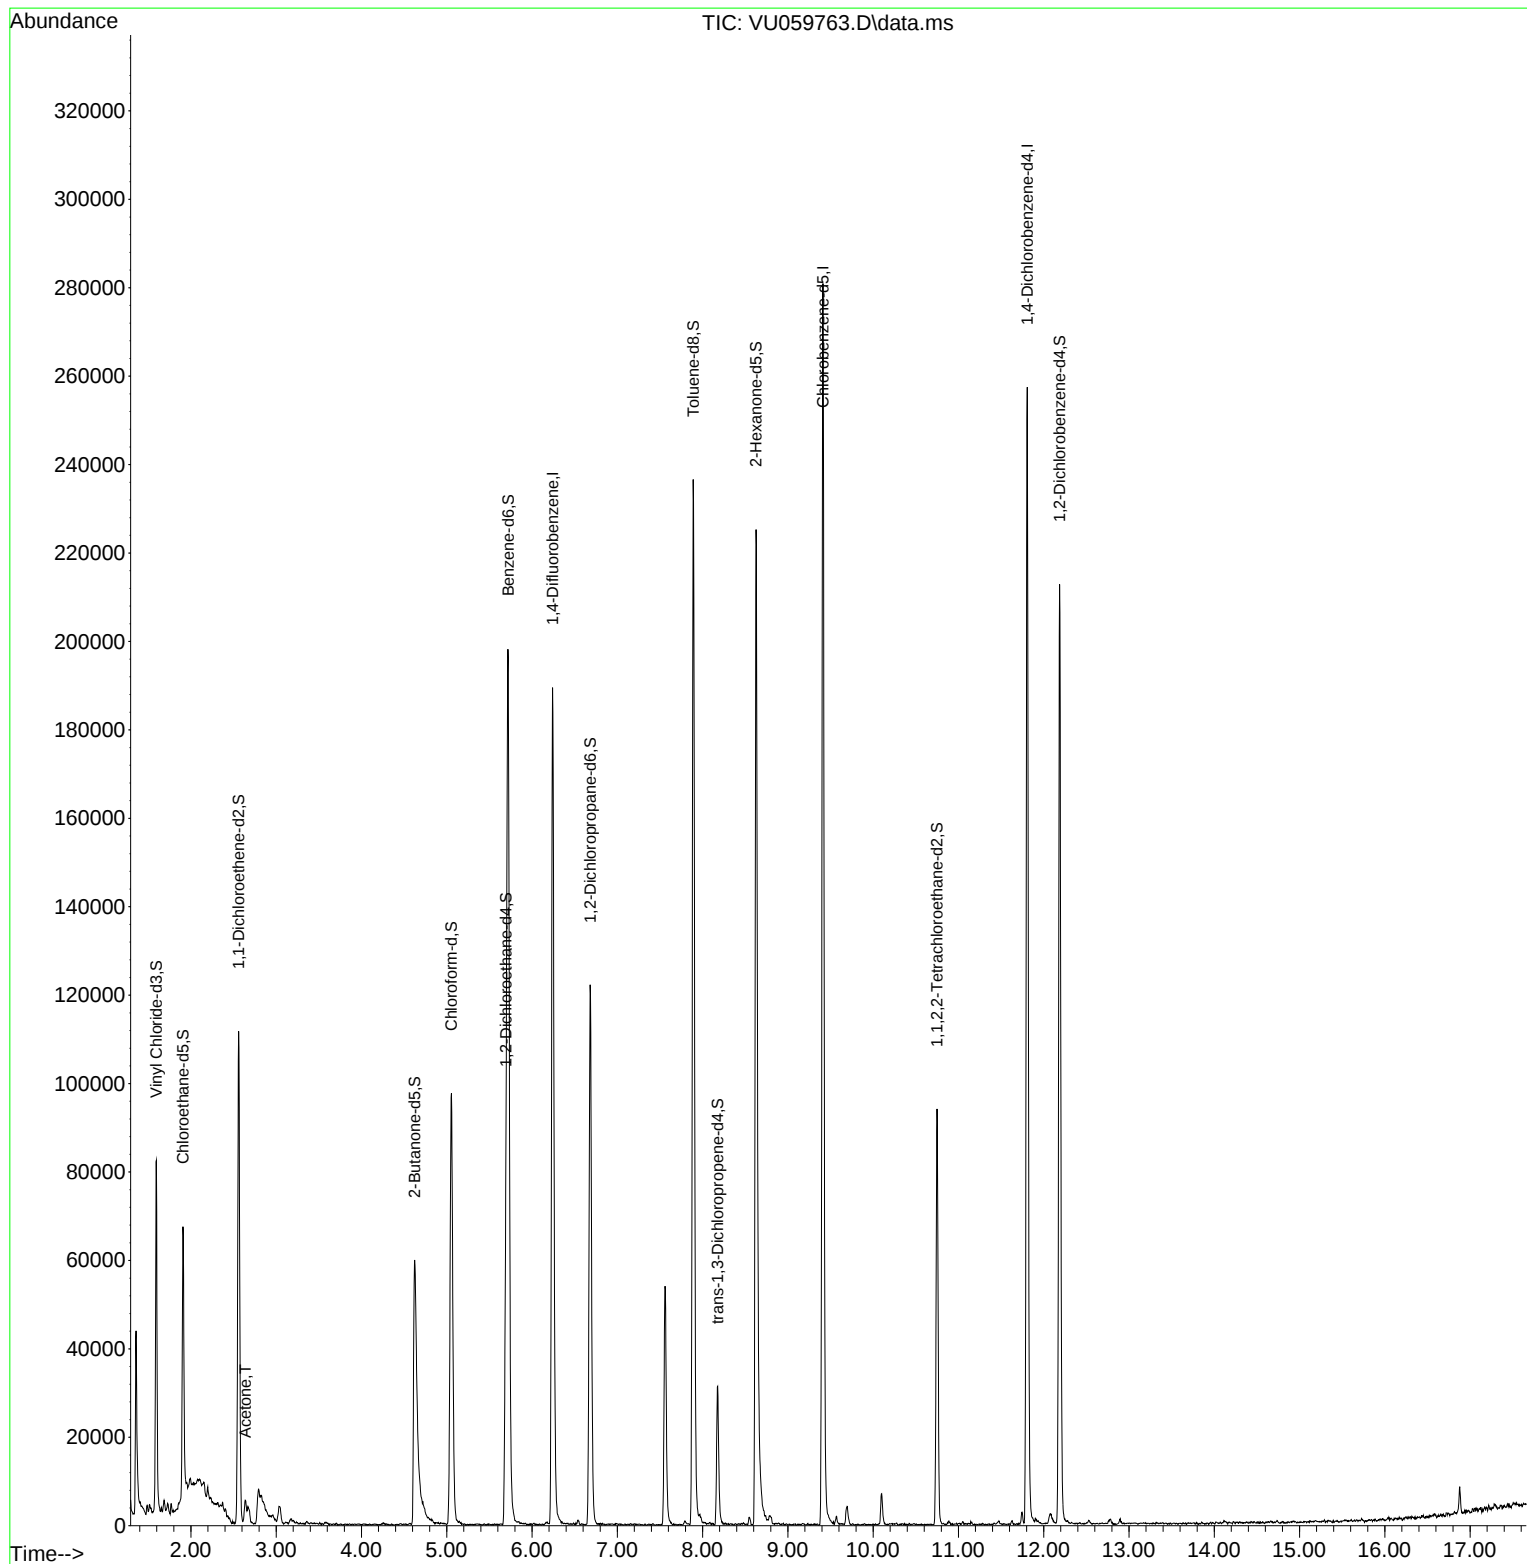

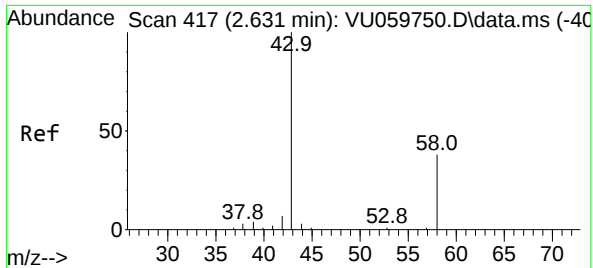

#13
 Acetone
 Concen: 5.477 ug/L
 RT: 2.637 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: VU059763.D
 Acq: 03 Jul 2024 01:33

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BK2

Tgt Ion: 43 Resp: 8297
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 68.0

