

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059780.D
 Acq On : 03 Jul 2024 08:16
 Operator : MD/SY
 Sample : P3122-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BP5

Quant Time: Jul 04 00:55:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 03 06:10:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	163418	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	168061	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	74357	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	52850	4.651	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.000%
7) Chloroethane-d5	1.907	69	46147	4.221	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.400%
11) 1,1-Dichloroethene-d2	2.560	65	19953	4.232	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.600%
20) 2-Butanone-d5	4.621	46	100069	42.752	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.500%
24) Chloroform-d	5.055	84	94150	4.037	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.800%
26) 1,2-Dichloroethane-d4	5.695	65	47818	4.256	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.721	84	196374	4.246	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.000%
36) 1,2-Dichloropropane-d6	6.682	67	61364	4.330	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.600%
41) Toluene-d8	7.891	98	169811	3.949	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
43) trans-1,3-Dichloroprop...	8.174	79	18859	4.249	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.624	63	80543	43.678	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.360%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	48413	4.134	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	61204	4.625	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.400%
Target Compounds						
					Qvalue	
13) Acetone	2.631	43	48496	31.940	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059780.D
Acq On : 03 Jul 2024 08:16
Operator : MD/SY
Sample : P3122-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BP5

Quant Time: Jul 04 00:55:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 03 06:10:28 2024
Response via : Initial Calibration

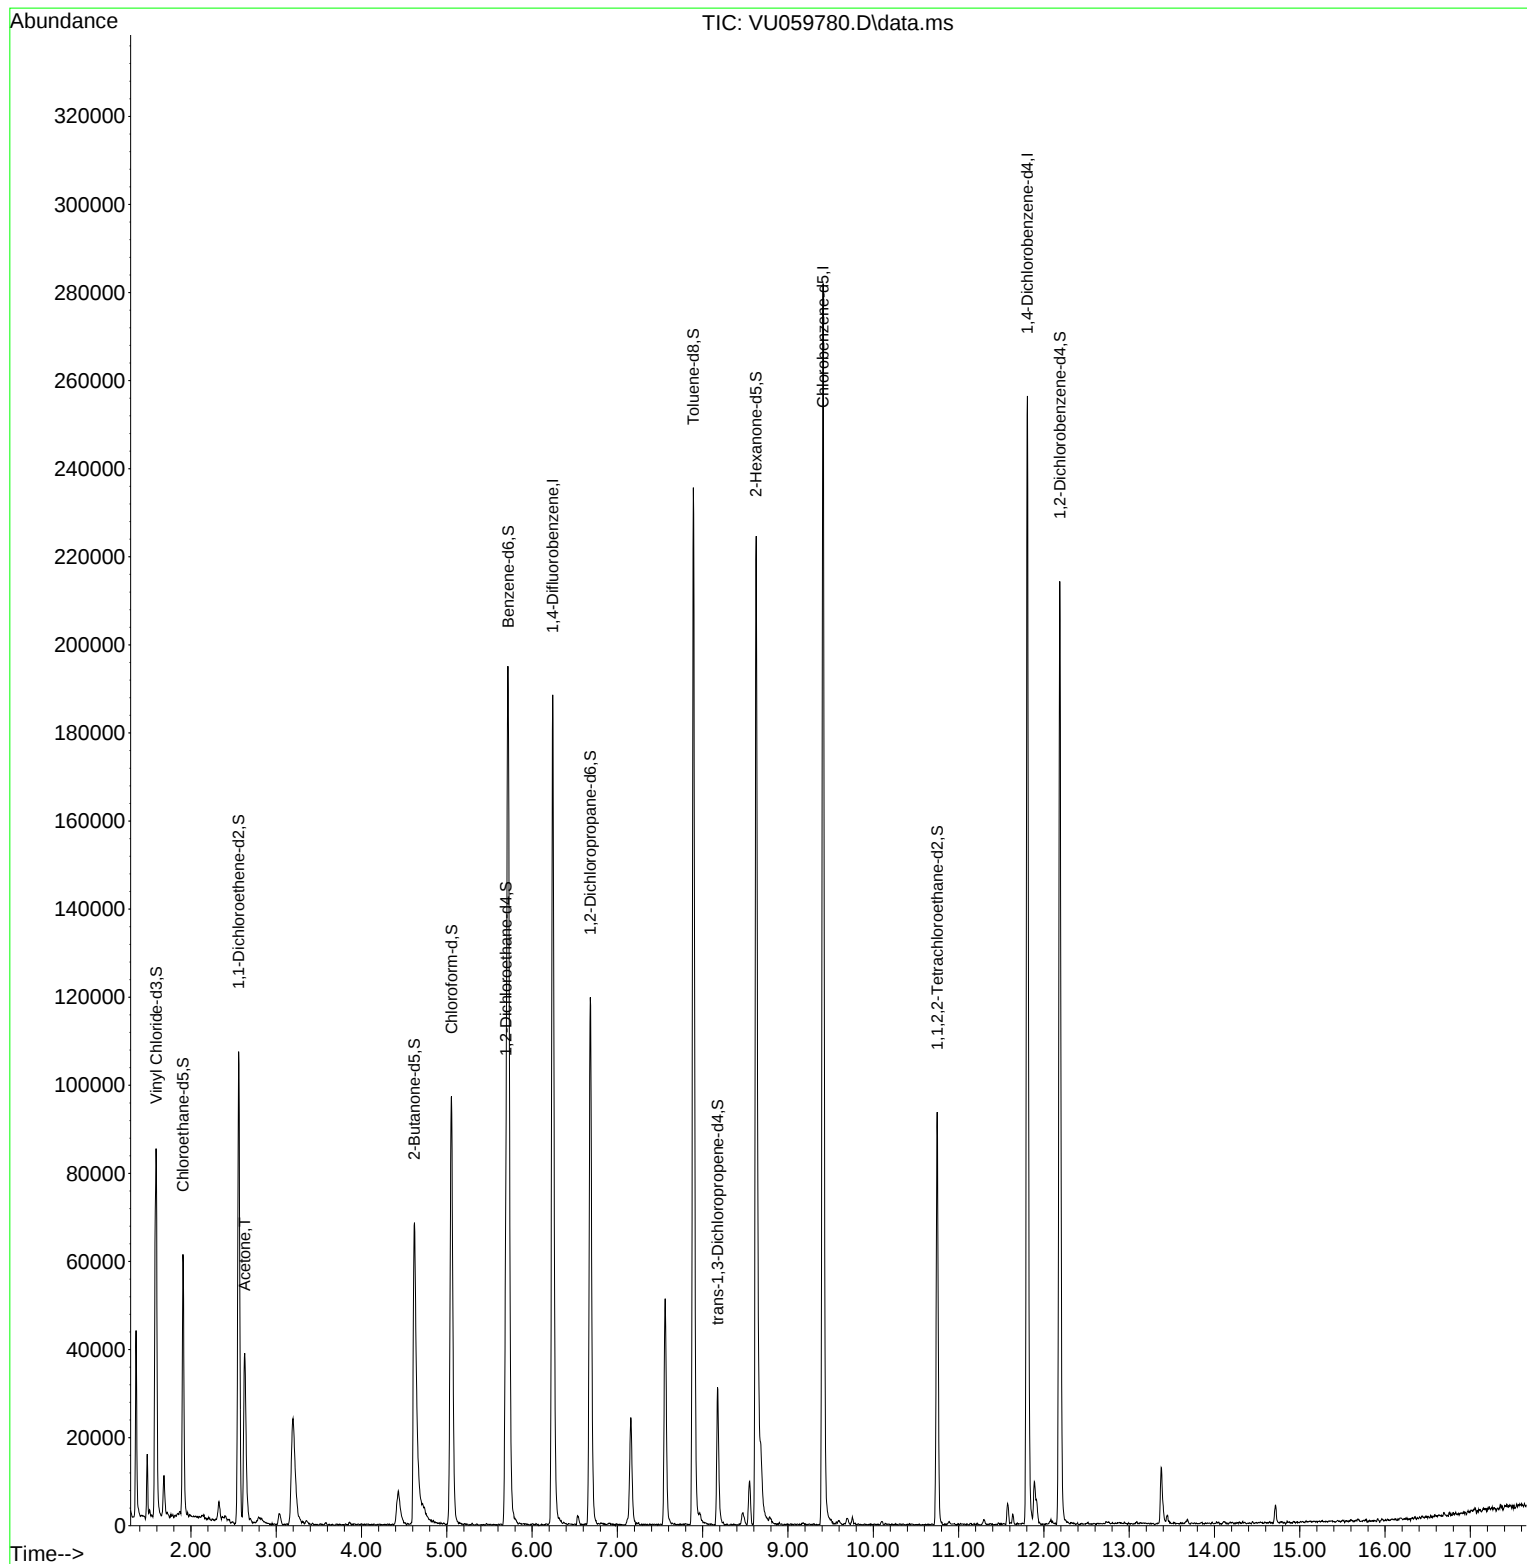

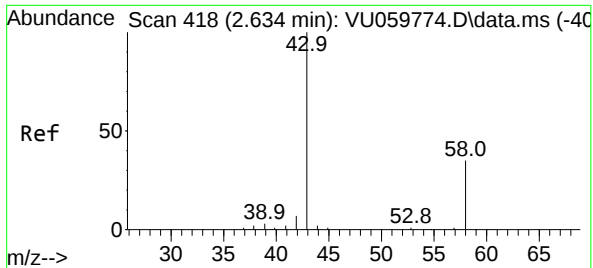

#13
 Acetone
 Concen: 31.940 ug/L
 RT: 2.631 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU059780.D
 Acq: 03 Jul 2024 08:16

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BP5

Tgt Ion: 43 Resp: 48496
 Ion Ratio Lower Upper
 43 100
 58 38.6 0.0 68.0

