

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059784.D
Acq On : 03 Jul 2024 09:52
Operator : MD/SY
Sample : P3060-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.447	345	360	385	rBV	1876600	3038607	7.02%	6.297%
2	2.798	442	469	535	rBV2	13544598	43311569	100.00%	89.757%
3	5.717	1359	1377	1398	rBV2	206163	533334	1.23%	1.105%
4	7.891	2040	2053	2070	rBV	247982	437144	1.01%	0.906%
5	8.627	2265	2282	2319	rBV	245642	460321	1.06%	0.954%
6	9.412	2513	2526	2543	rBV	284661	473290	1.09%	0.981%




Sum of corrected areas: 48254265

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059784.D
Acq On : 03 Jul 2024 09:52
Operator : MD/SY
Sample : P3060-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

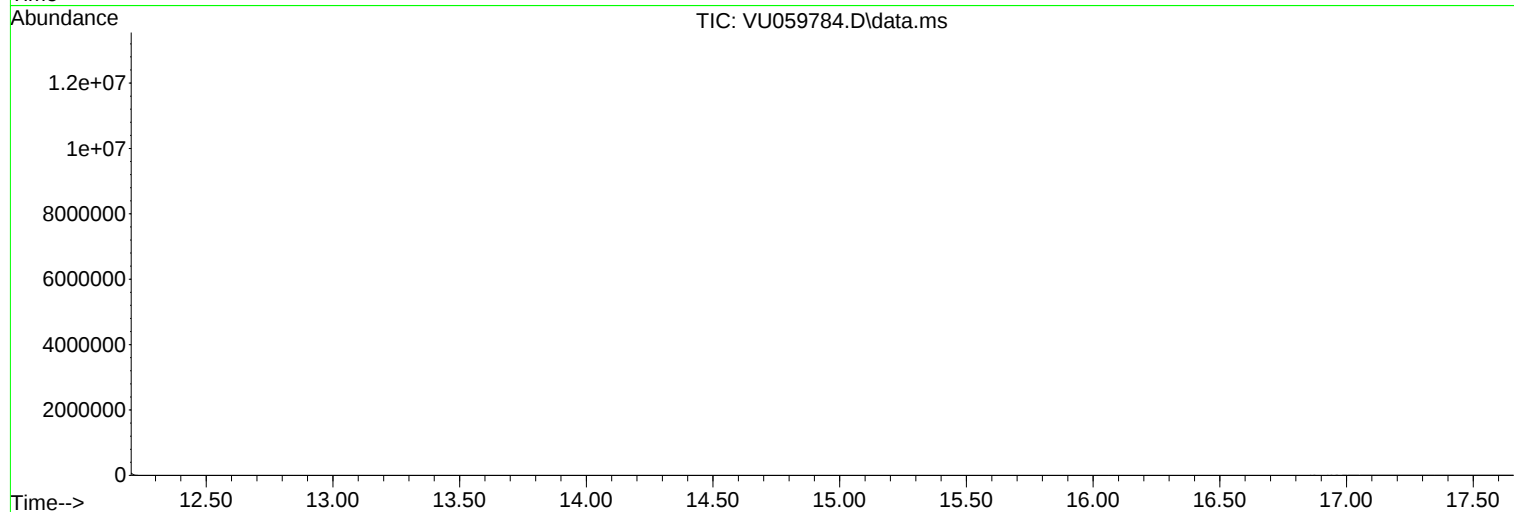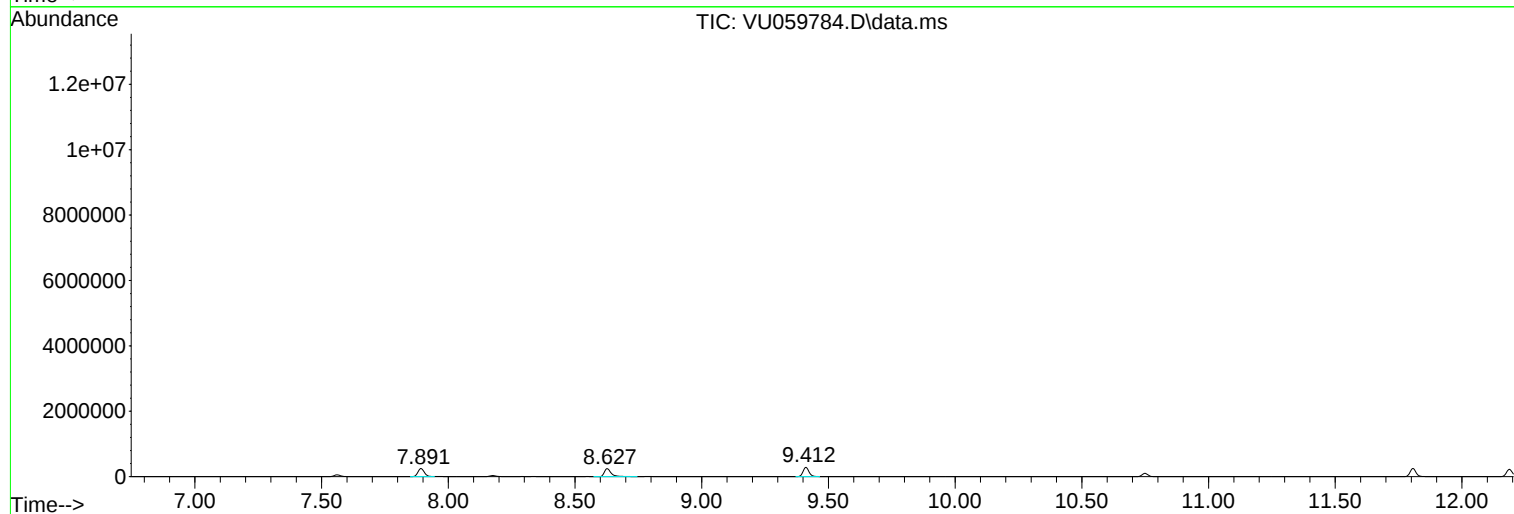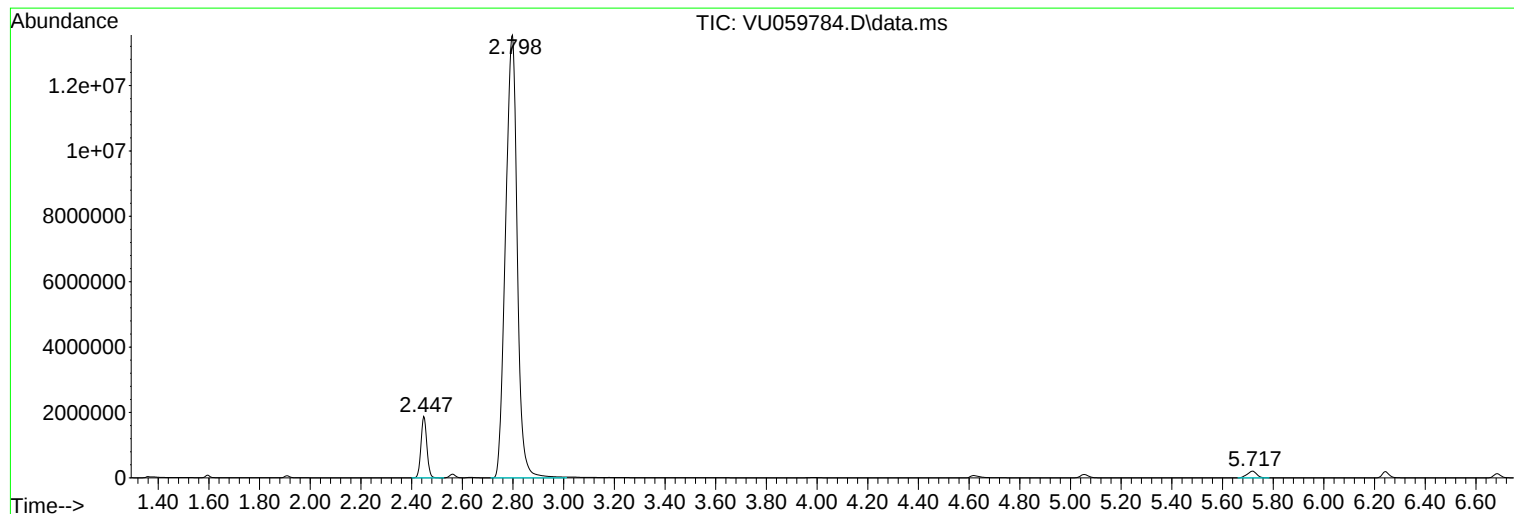

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059784.D
Acq On : 03 Jul 2024 09:52
Operator : MD/SY
Sample : P3060-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP7









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	28.49 ug/L	3038610	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

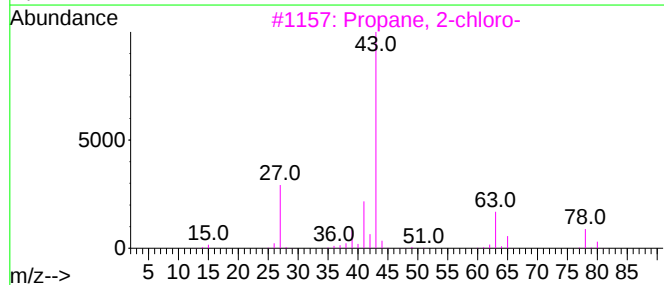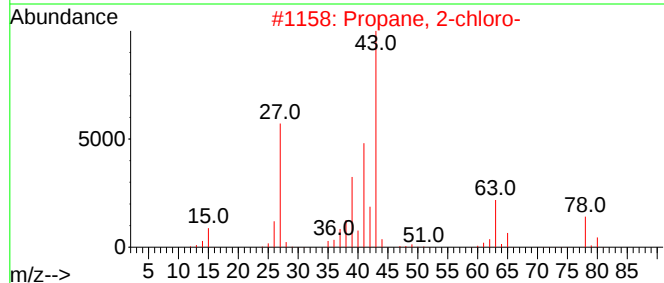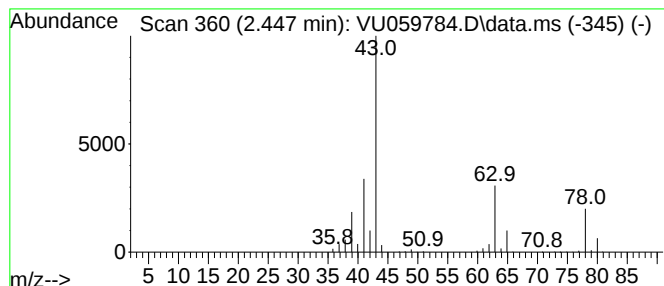

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059784.D
Acq On : 03 Jul 2024 09:52
Operator : MD/SY
Sample : P3060-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.798	406.05 ug/L	43311600	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	90
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	83
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

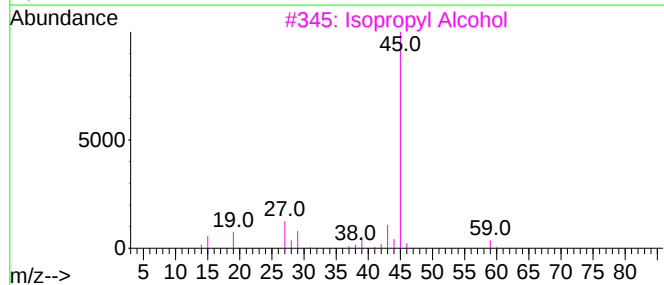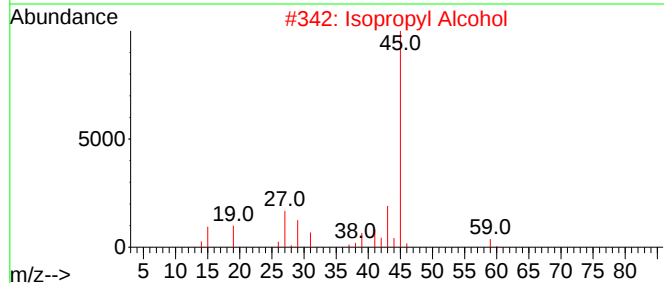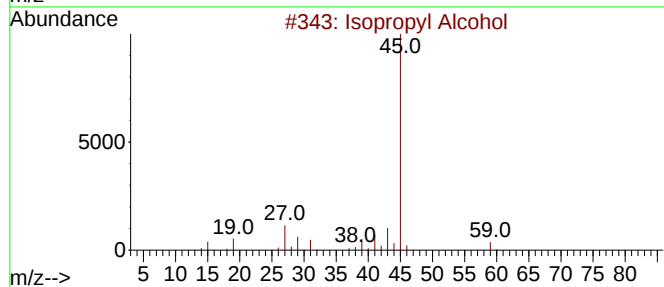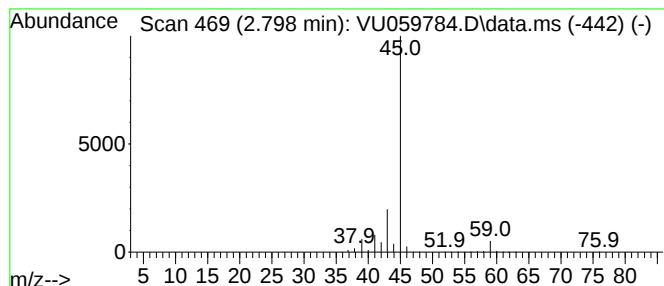

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059784.D
Acq On : 03 Jul 2024 09:52
Operator : MD/SY
Sample : P3060-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	28.5	ug/L	3038610	1	6.242	533334	5.0
Isopropyl Alcohol	2.798	406.1	ug/L	43311600	1	6.242	533334	5.0