

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059785.D
Acq On : 03 Jul 2024 10:16
Operator : MD/SY
Sample : P3060-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	347	360	378	rVB	451525	735607	2.02%	1.872%
2	2.792	443	467	534	rBV	11511537	36368488	100.00%	92.561%
3	5.718	1358	1377	1401	rBV2	192613	496069	1.36%	1.263%
4	7.891	2040	2053	2070	rBV	230090	399029	1.10%	1.016%
5	8.627	2271	2282	2310	rBV	221329	418266	1.15%	1.065%
6	9.412	2512	2526	2548	rBV	278768	464828	1.28%	1.183%
7	11.807	3259	3271	3292	rBV	250563	408930	1.12%	1.041%




Sum of corrected areas: 39291217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059785.D
Acq On : 03 Jul 2024 10:16
Operator : MD/SY
Sample : P3060-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

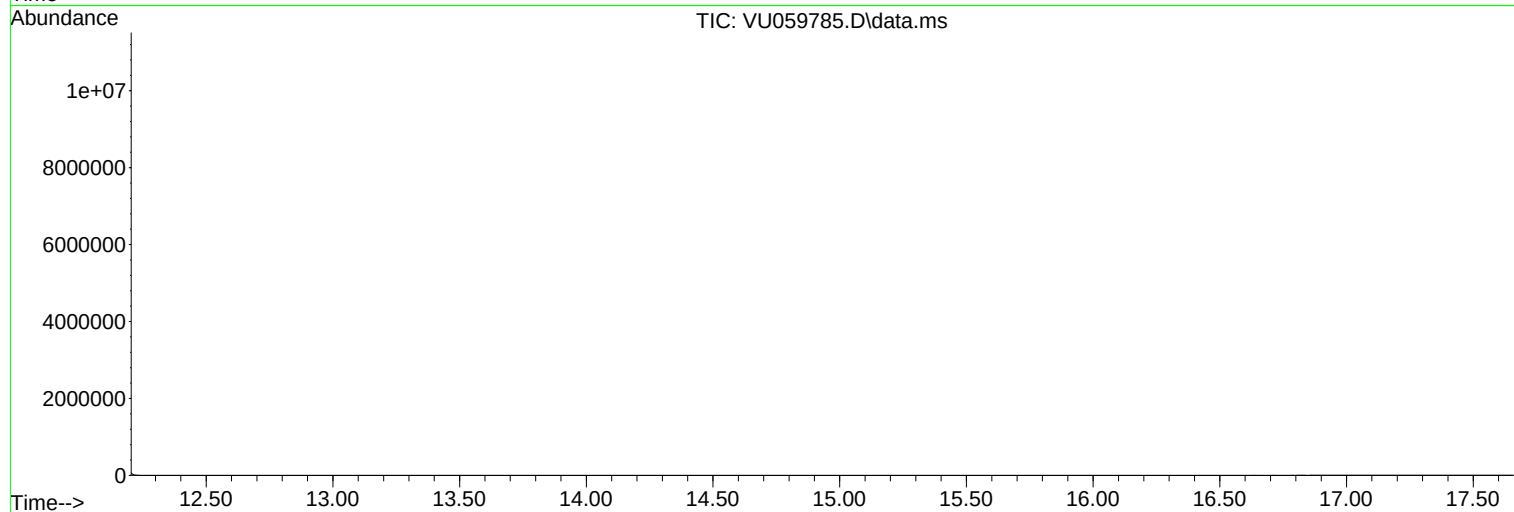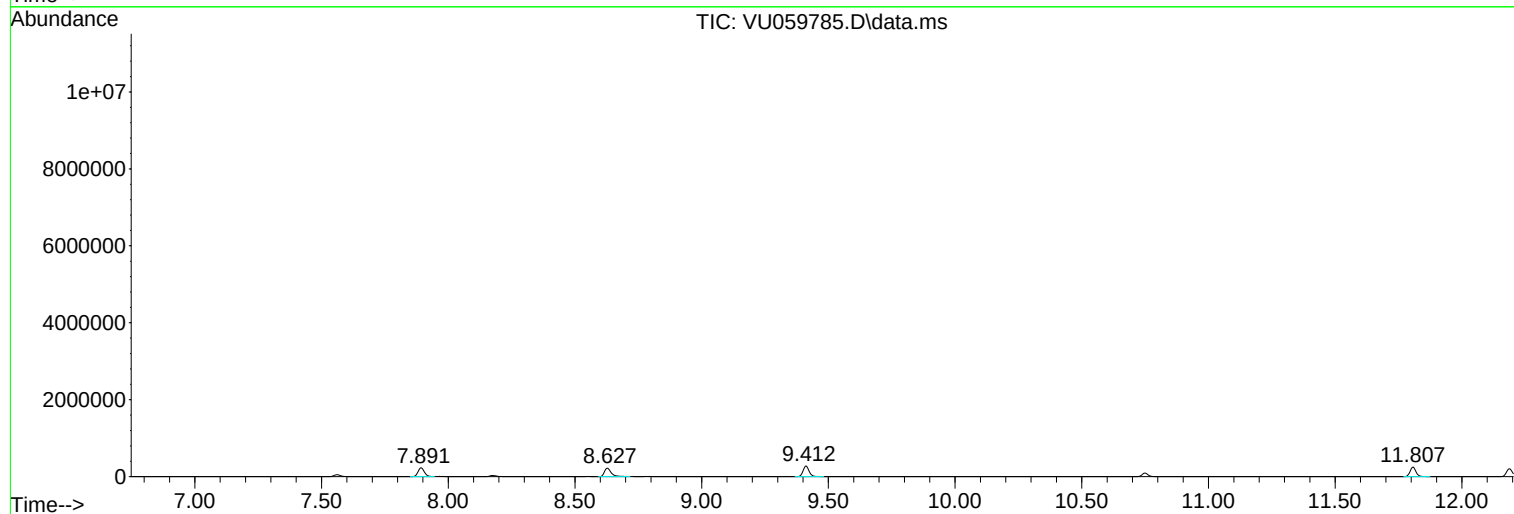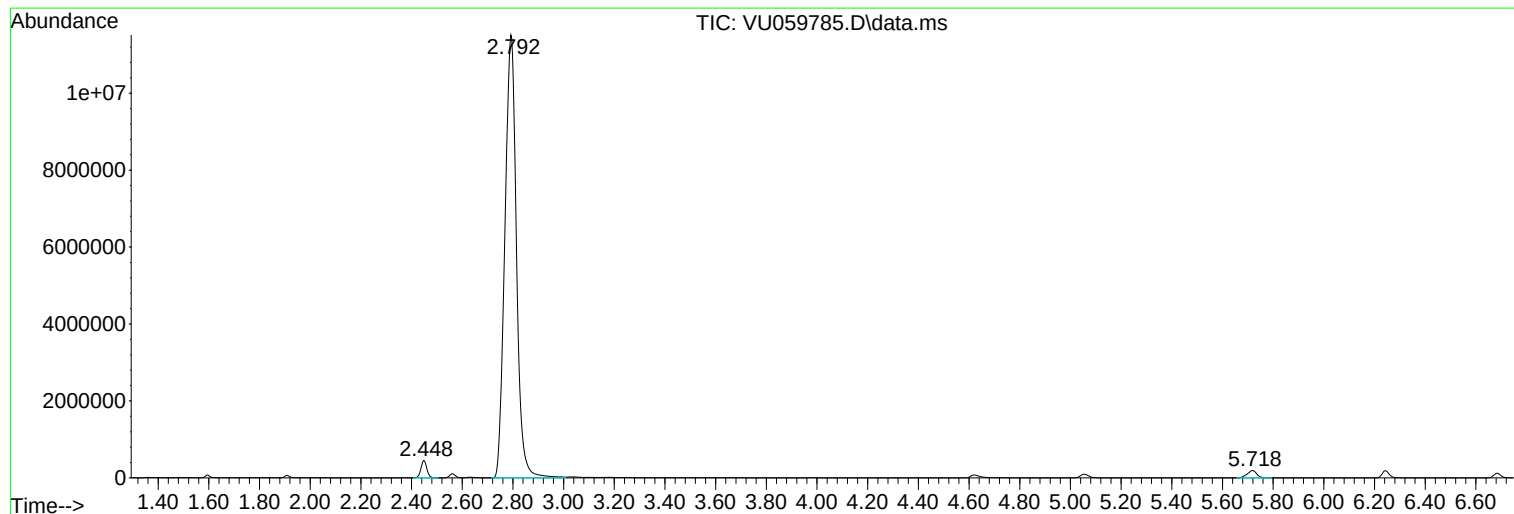

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059785.D
Acq On : 03 Jul 2024 10:16
Operator : MD/SY
Sample : P3060-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	7.41 ug/L	735607	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	45
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

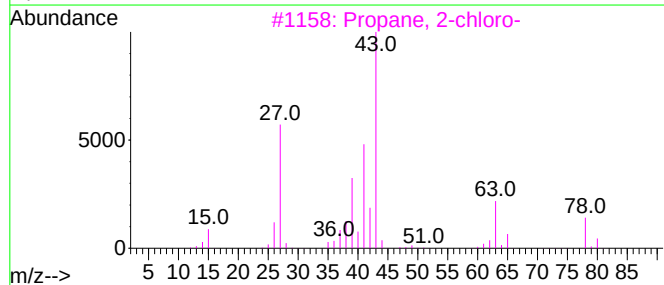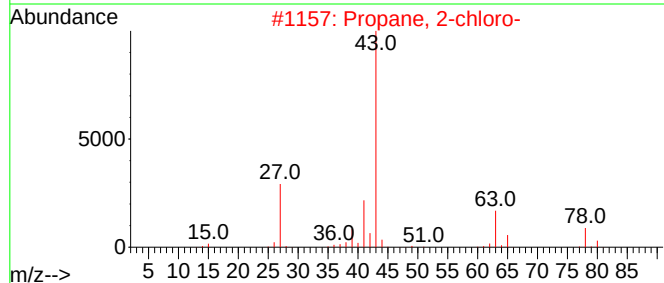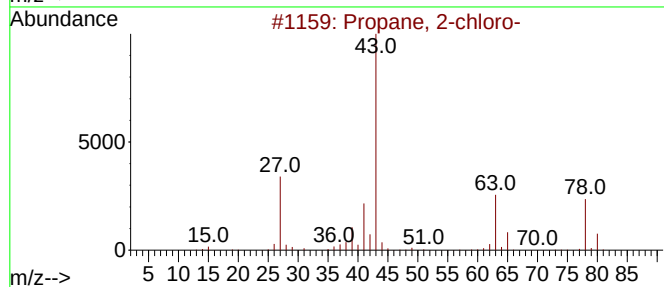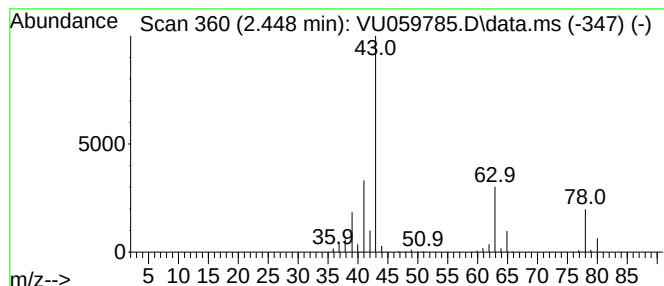

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059785.D
Acq On : 03 Jul 2024 10:16
Operator : MD/SY
Sample : P3060-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.792	366.57 ug/L	36368500	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

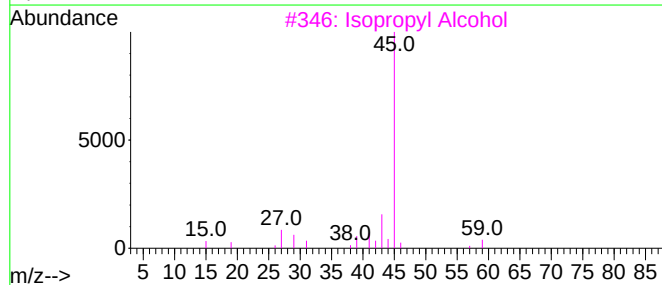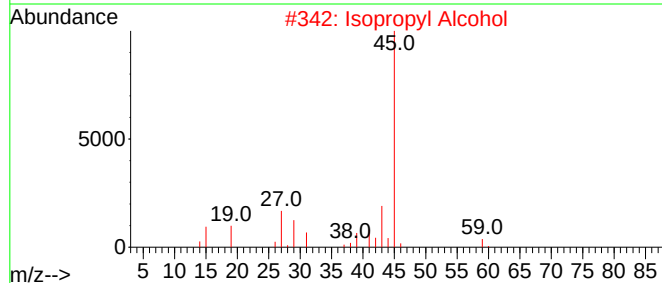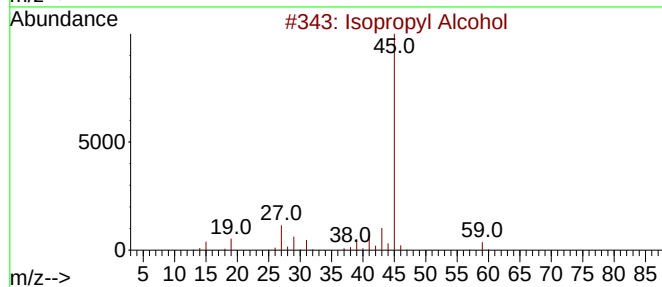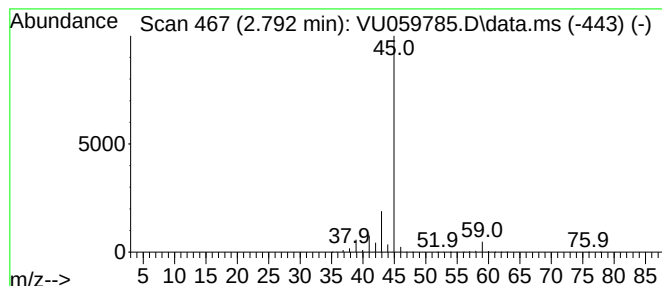

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059785.D
Acq On : 03 Jul 2024 10:16
Operator : MD/SY
Sample : P3060-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	7.4	ug/L	735607	1	6.242	496069	5.0
Isopropyl Alcohol	2.792	366.6	ug/L	36368500	1	6.242	496069	5.0