

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059788.D
 Acq On : 03 Jul 2024 11:25
 Operator : MD/SY
 Sample : P3084-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G74

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU059788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	84	95	110	rBV3	97059	128669	1.35%	0.902%
2	2.448	348	360	382	rVB	427390	692368	7.29%	4.854%
3	2.560	382	395	408	rBV	109897	182238	1.92%	1.278%
4	2.782	444	464	533	rBV	3047154	9497593	100.00%	66.586%
5	4.618	1022	1035	1040	rBV2	69304	129111	1.36%	0.905%
6	5.055	1155	1171	1194	rBV2	100379	237970	2.51%	1.668%
7	5.718	1357	1377	1410	rBV2	197014	517883	5.45%	3.631%
8	6.242	1528	1540	1560	rBV	178014	342551	3.61%	2.402%
9	6.682	1660	1677	1693	rBV	122037	235357	2.48%	1.650%
10	7.560	1937	1950	1972	rBV	55002	100589	1.06%	0.705%
11	7.891	2041	2053	2068	rBV	233429	405543	4.27%	2.843%
12	8.627	2271	2282	2319	rBV	225100	434512	4.57%	3.046%
13	9.412	2511	2526	2549	rBV	269307	453642	4.78%	3.180%
14	10.750	2931	2942	2957	rBV2	92662	151920	1.60%	1.065%
15	11.807	3259	3271	3295	rBV	240796	398913	4.20%	2.797%
16	12.187	3377	3389	3407	rBV	213406	354709	3.73%	2.487%




Sum of corrected areas: 14263568

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059788.D
Acq On : 03 Jul 2024 11:25
Operator : MD/SY
Sample : P3084-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

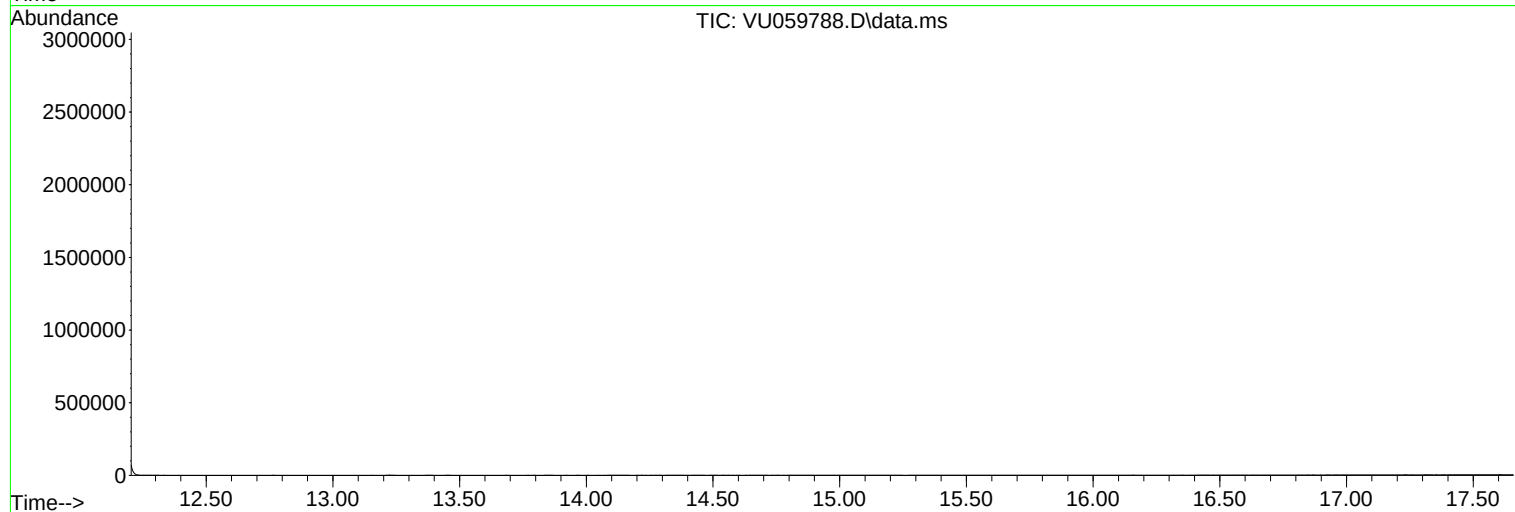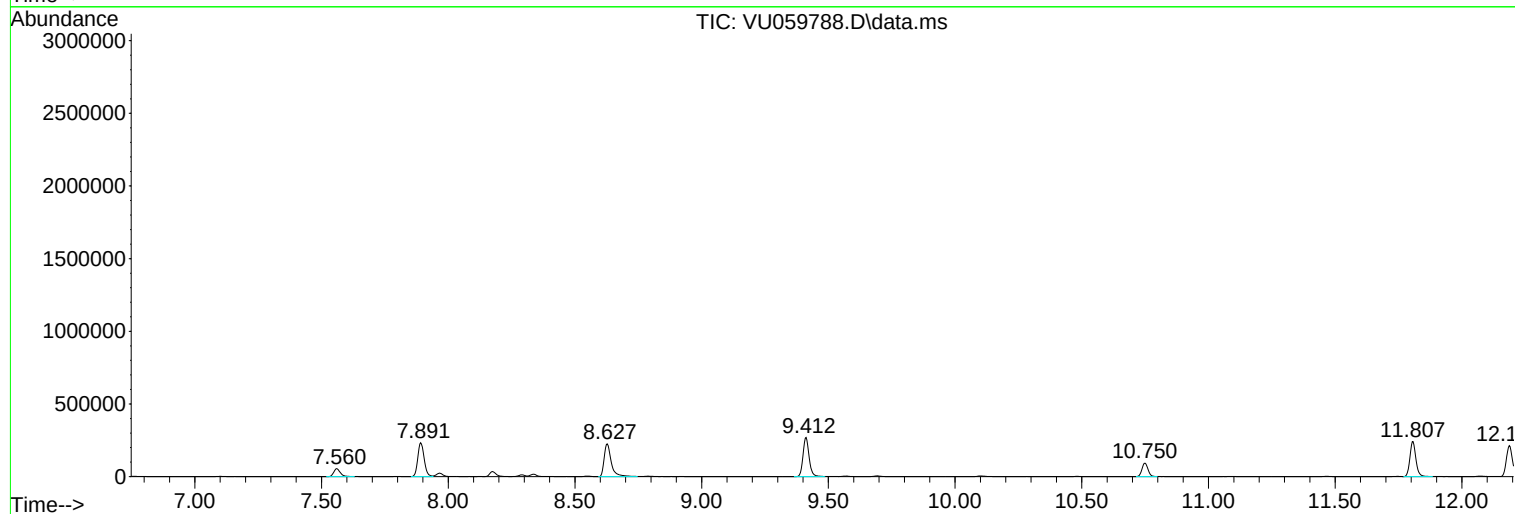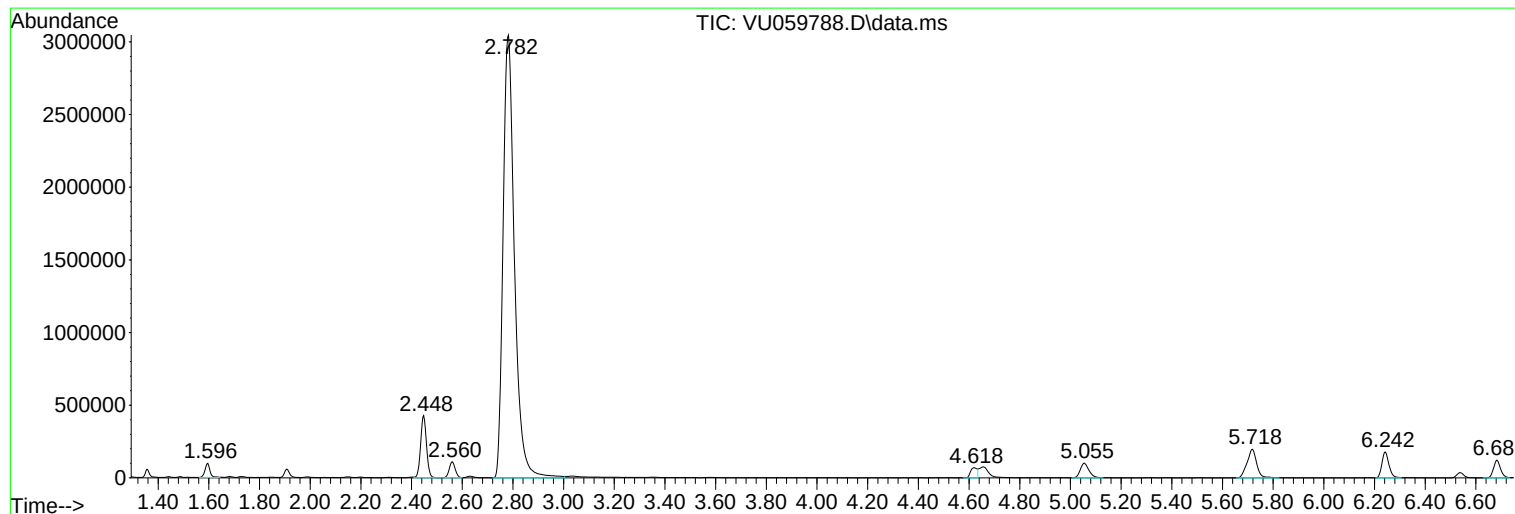

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059788.D
Acq On : 03 Jul 2024 11:25
Operator : MD/SY
Sample : P3084-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G74










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	10.11 ug/L	692368	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	59
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

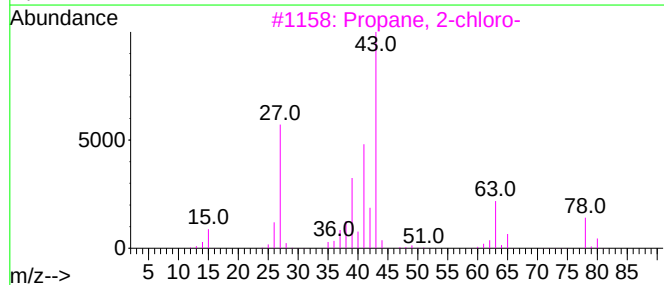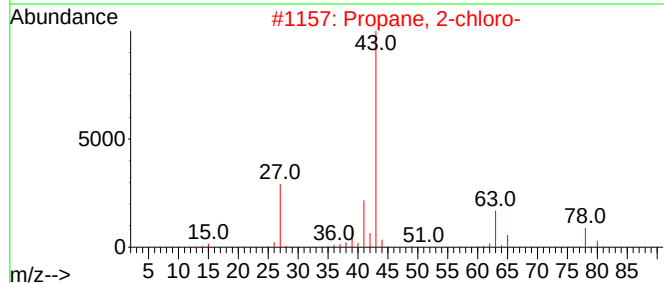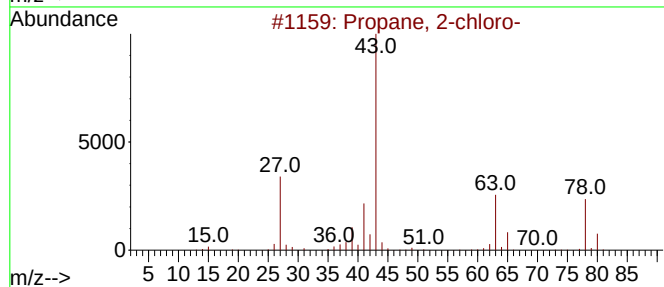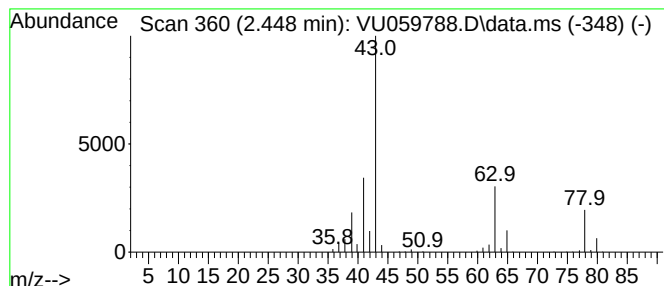

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059788.D
Acq On : 03 Jul 2024 11:25
Operator : MD/SY
Sample : P3084-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G74










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.782	138.63 ug/L	9497590	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

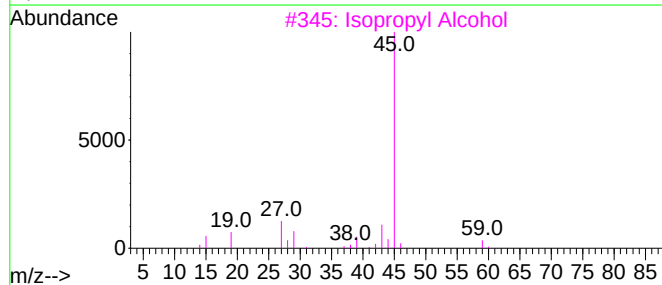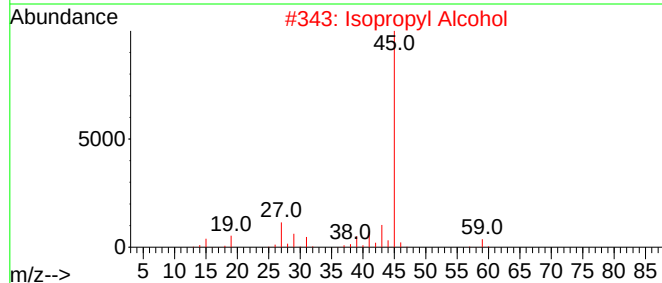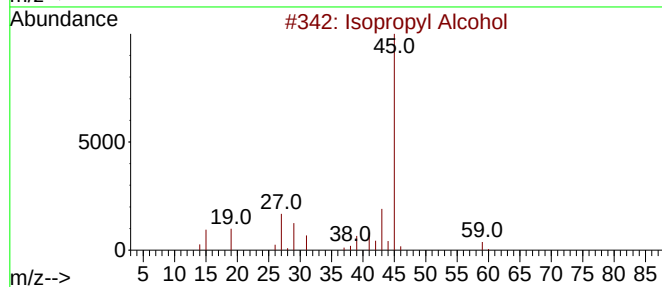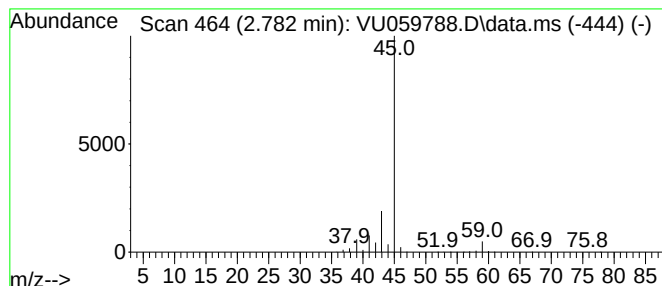

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059788.D
Acq On : 03 Jul 2024 11:25
Operator : MD/SY
Sample : P3084-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	10.1	ug/L	692368	1	6.242	342551	5.0
Isopropyl Alcohol	2.782	138.6	ug/L	9497590	1	6.242	342551	5.0