

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059792.D
 Acq On : 03 Jul 2024 12:56
 Operator : MD/SY
 Sample : P3099-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU059792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.461	48	53	59	rBV2	7518	7215	1.52%	0.178%
2	1.596	87	95	115	rVB	68092	82969	17.47%	2.052%
3	1.907	183	192	206	rBV	54455	71828	15.13%	1.776%
4	2.560	382	395	410	rBV	101468	165126	34.77%	4.084%
5	2.785	452	465	482	rBV	8942	26046	5.49%	0.644%
6	3.039	534	544	554	rBV4	3826	6970	1.47%	0.172%
7	4.618	1025	1035	1061	rBV	60480	155605	32.77%	3.848%
8	5.055	1155	1171	1194	rBV	93299	213628	44.99%	5.283%
9	5.718	1356	1377	1399	rBV2	181975	474849	100.00%	11.743%
10	6.242	1527	1540	1567	rBV	175599	340819	71.77%	8.428%
11	6.682	1665	1677	1697	rBV	112698	220950	46.53%	5.464%
12	7.560	1939	1950	1968	rBV2	52808	94655	19.93%	2.341%
13	7.891	2041	2053	2071	rBV	217448	382434	80.54%	9.457%
14	8.177	2130	2142	2163	rBV2	30811	54782	11.54%	1.355%
15	8.550	2251	2258	2267	rVB5	3376	5472	1.15%	0.135%
16	8.627	2269	2282	2321	rBV	211647	402089	84.68%	9.944%
17	9.412	2514	2526	2549	rBV	265615	444816	93.68%	11.000%
18	10.750	2930	2942	2956	rBV2	90069	143809	30.29%	3.556%
19	11.807	3259	3271	3299	rBV	238140	392092	82.57%	9.696%
20	12.065	3341	3351	3363	rBV3	9987	22239	4.68%	0.550%
21	12.187	3377	3389	3409	rBV	196404	335330	70.62%	8.293%




Sum of corrected areas: 4043723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059792.D
Acq On : 03 Jul 2024 12:56
Operator : MD/SY
Sample : P3099-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

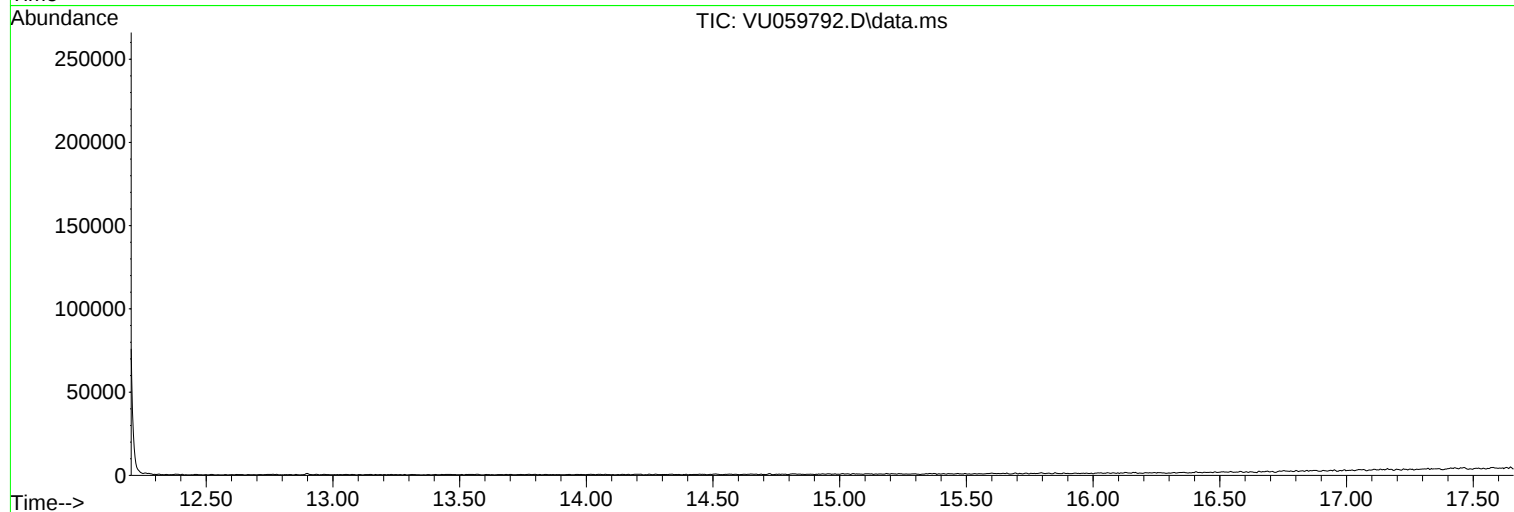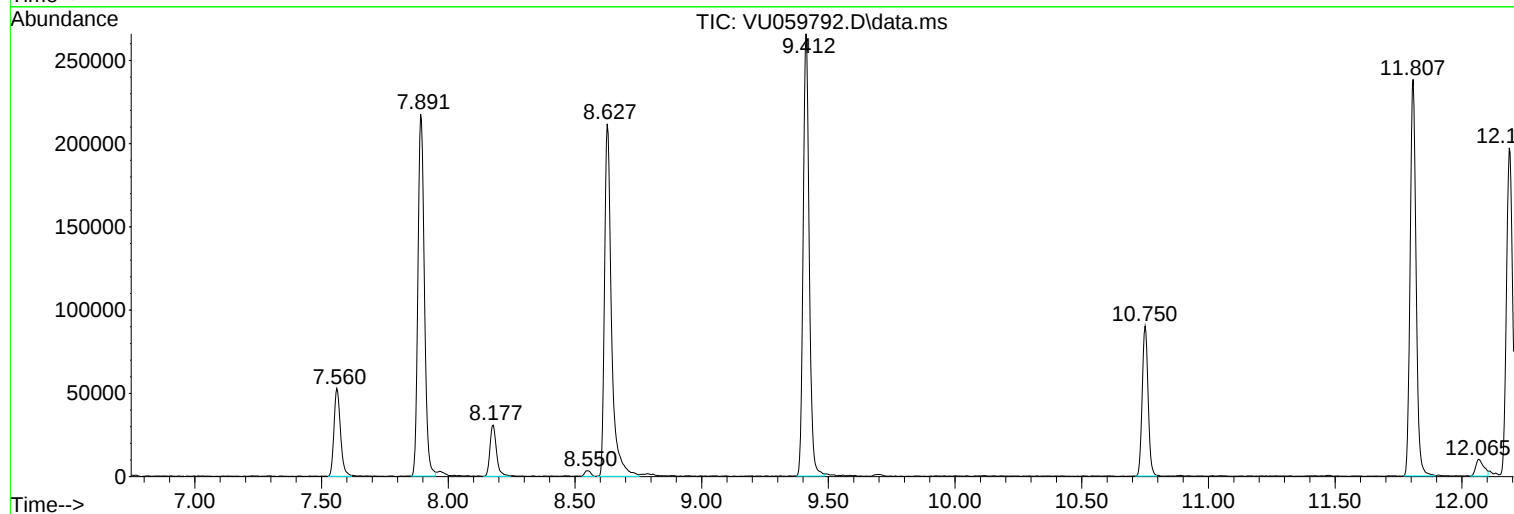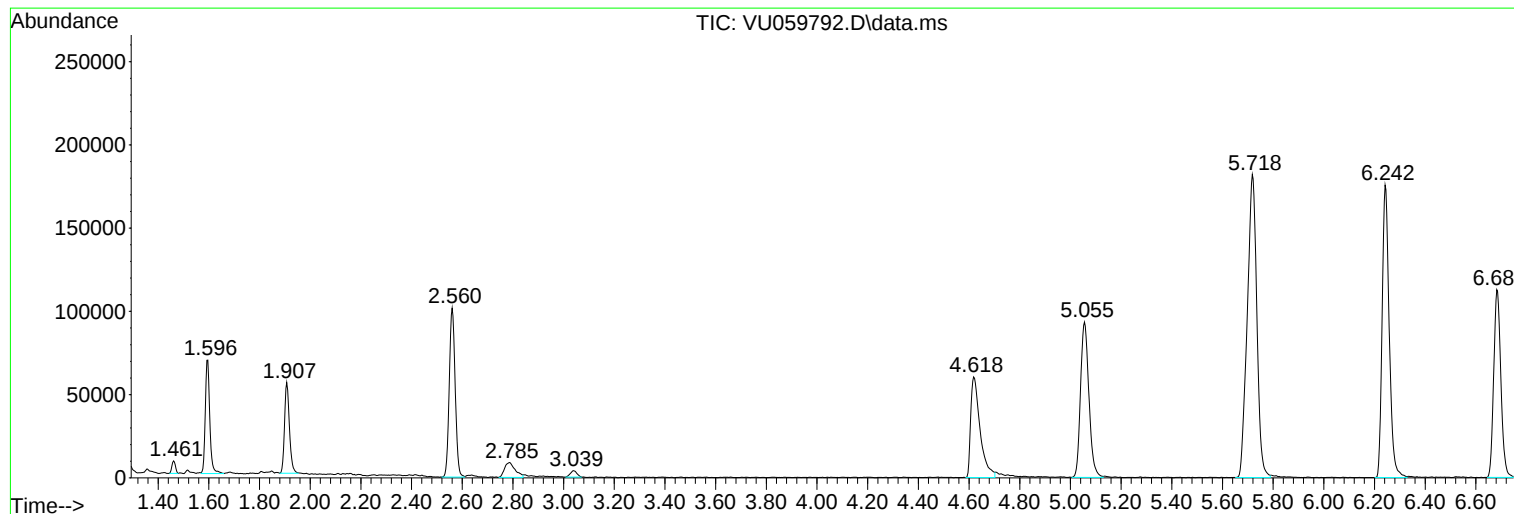

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059792.D
Acq On : 03 Jul 2024 12:56
Operator : MD/SY
Sample : P3099-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059792.D
Acq On : 03 Jul 2024 12:56
Operator : MD/SY
Sample : P3099-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc