

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
 Data File : VU059831.D
 Acq On : 04 Jul 2024 05:16
 Operator : MD/SY
 Sample : P3137-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZH3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	109	rVB	75186	93187	8.23%	1.554%
2	1.907	183	192	205	rBV	59956	80407	7.10%	1.341%
3	2.560	384	395	412	rBV	111964	187549	16.57%	3.127%
4	4.657	1026	1047	1081	rBV3	121314	438408	38.73%	7.311%
5	5.055	1156	1171	1196	rBV	105046	231664	20.47%	3.863%
6	5.718	1357	1377	1407	rBV3	213218	555020	49.04%	9.255%
7	6.242	1528	1540	1572	rBV	197120	383040	33.84%	6.387%
8	6.534	1617	1631	1664	rBV	602561	1131854	100.00%	18.874%
9	6.682	1665	1677	1701	rVB	130776	257440	22.74%	4.293%
10	7.560	1939	1950	1972	rBV2	57760	106896	9.44%	1.783%
11	7.891	2041	2053	2074	rBV	257792	451426	39.88%	7.528%
12	8.174	2132	2141	2167	rBV	33844	61524	5.44%	1.026%
13	8.306	2174	2182	2196	rVB4	7409	11708	1.03%	0.195%
14	8.550	2246	2258	2268	rBV3	14077	23244	2.05%	0.388%
15	8.627	2271	2282	2317	rBV	249671	488711	43.18%	8.150%
16	9.412	2513	2526	2552	rBV	286013	496319	43.85%	8.276%
17	10.750	2925	2942	2960	rBV	101729	165467	14.62%	2.759%
18	11.807	3259	3271	3290	rBV	266605	437372	38.64%	7.293%
19	12.187	3372	3389	3406	rBV	240604	395551	34.95%	6.596%




Sum of corrected areas: 5996787

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059831.D
Acq On : 04 Jul 2024 05:16
Operator : MD/SY
Sample : P3137-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

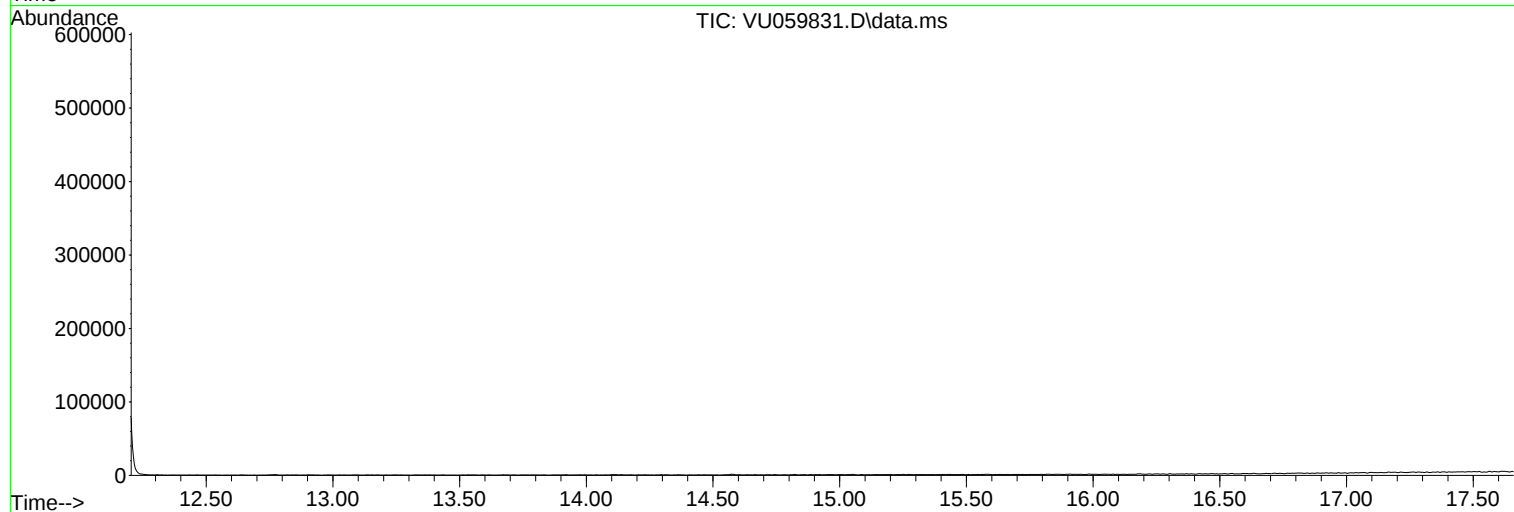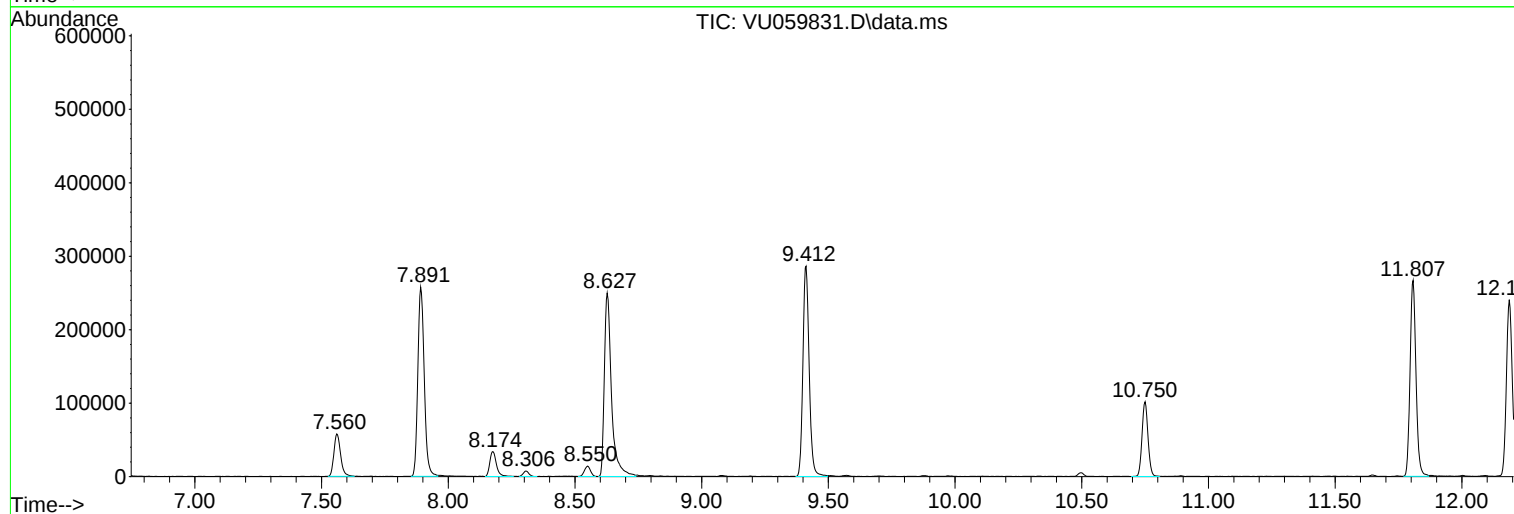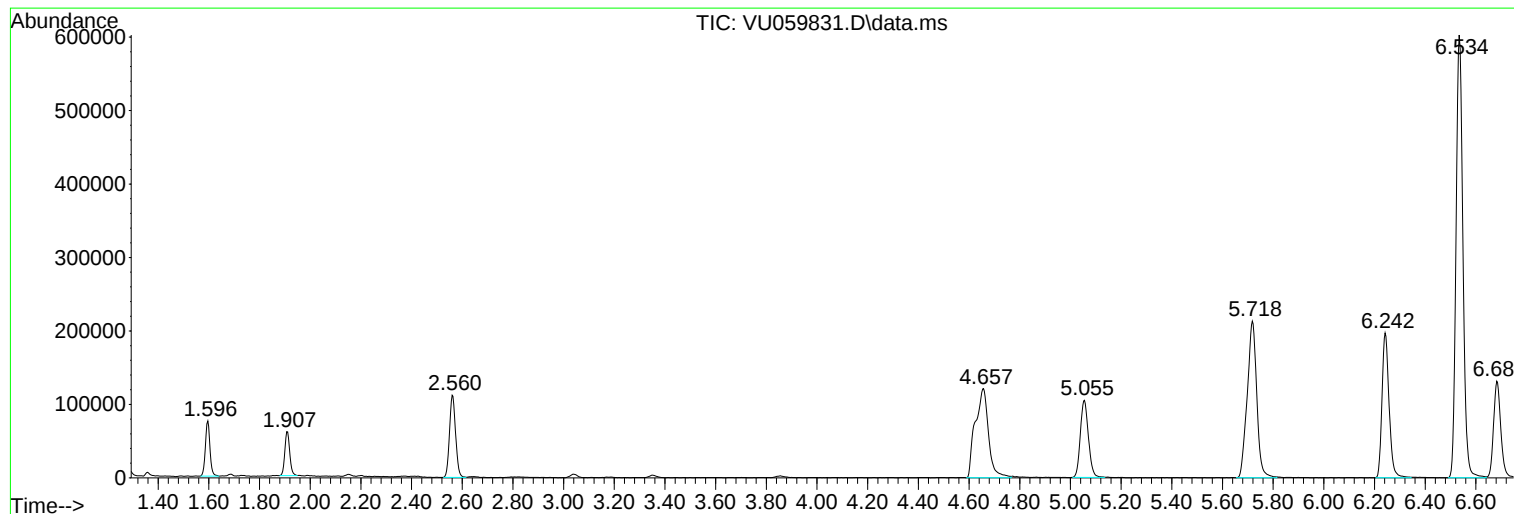

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059831.D
Acq On : 04 Jul 2024 05:16
Operator : MD/SY
Sample : P3137-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059831.D
Acq On : 04 Jul 2024 05:16
Operator : MD/SY
Sample : P3137-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc