


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070324\
Data File : VU059749.D
Acq On : 02 Jul 2024 19:27
Operator : MD/SY
Sample : BFB169
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB169

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jul 04 04:26:48 2024

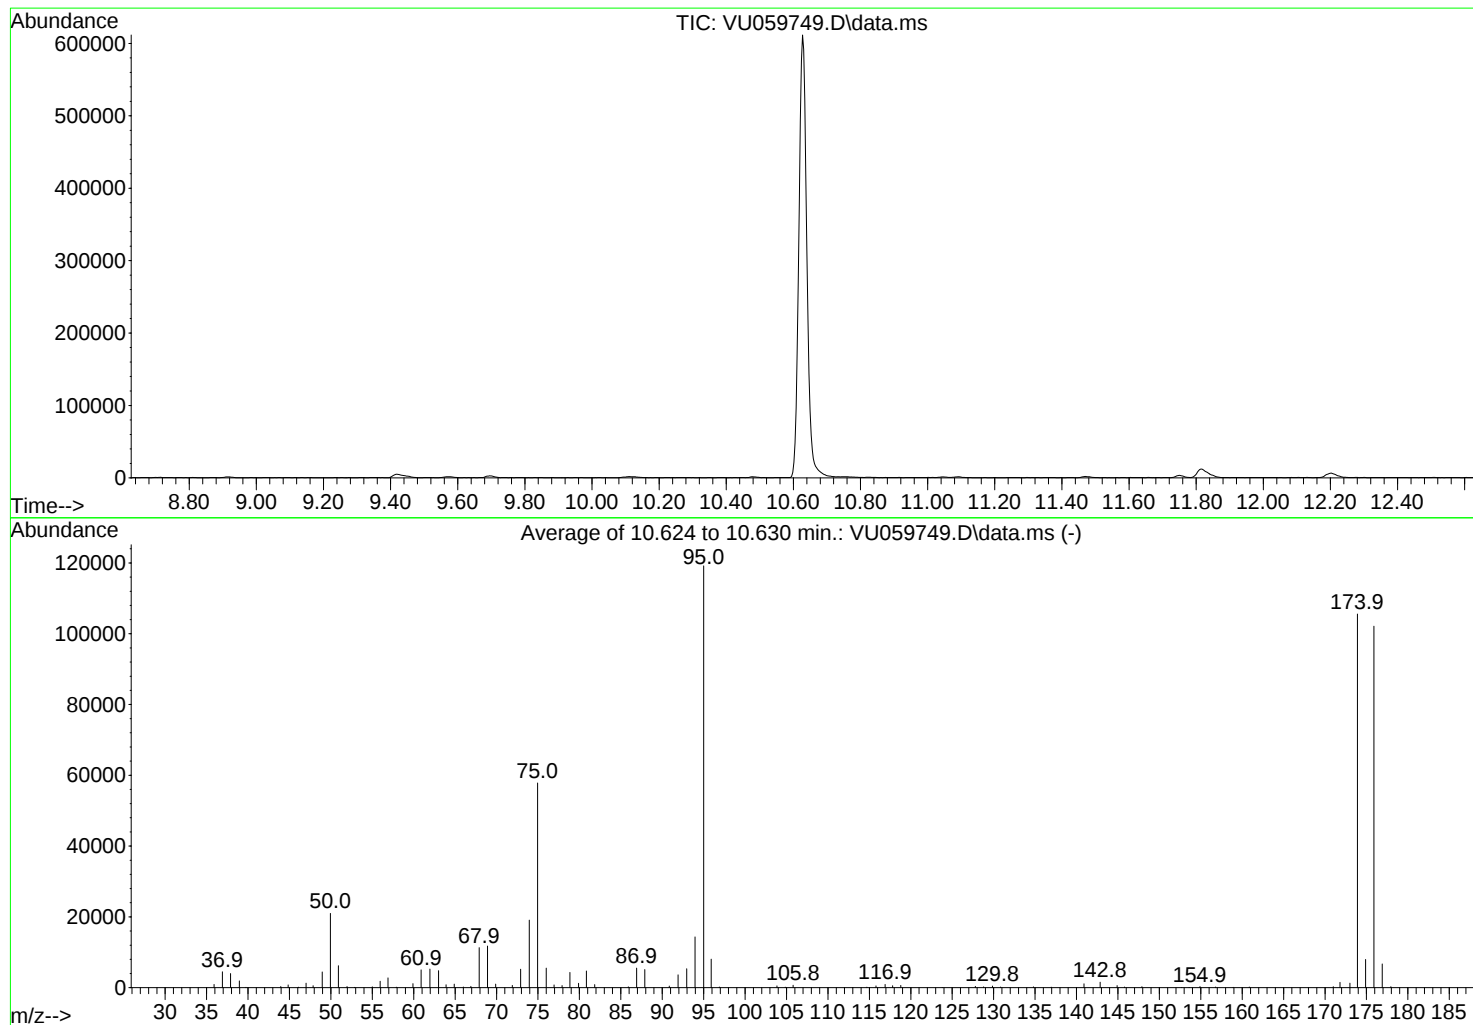

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	20992	PASS
75	95	30	80	48.5	57821	PASS
95	95	100	100	100.0	119184	PASS
96	95	5	9	6.8	8061	PASS
173	174	0.00	2	1.2	1290	PASS
174	95	50	120	88.6	105584	PASS
175	174	5	9	7.5	7948	PASS
176	174	95	101	96.7	102139	PASS
177	176	5	9	6.6	6709	PASS

m/z	Abundance
39.80	104.0
43.90	406.0

Instrument :
MSVOA_U
ClientSampleId :
BFB169

m/z	Abundance
35.90	890.0
36.90	4625.0
37.90	3952.0
39.00	1995.0
39.70	181.0
44.00	637.0
44.90	721.0
46.10	155.0
47.00	1246.0
47.90	541.0
48.90	4521.0
49.90	20696.0
50.90	6152.0
51.90	323.0
52.80	114.0
55.00	223.0
55.90	1760.0
56.90	2715.0
57.90	137.0
59.90	1149.0
60.90	5098.0
61.90	5403.0
63.00	4665.0
63.90	835.0
64.90	1011.0
66.00	195.0
66.90	362.0
67.90	11128.0
68.90	11254.0
69.90	1112.0
71.90	564.0
72.90	5021.0
74.00	18976.0
75.00	56768.0
76.00	5594.0
76.90	719.0
77.90	523.0
78.90	4235.0
79.90	1240.0
80.90	4634.0
81.90	876.0
85.90	216.0
86.90	5340.0
87.90	5222.0
90.80	412.0
91.90	3555.0
92.90	5261.0
93.90	14058.0
95.00	115400.0
95.90	8119.0
96.90	209.0
103.80	482.0
104.80	135.0
105.80	666.0
114.70	124.0
115.80	469.0
116.90	890.0
117.80	533.0
118.80	573.0
127.80	287.0
128.80	228.0
129.90	468.0
130.80	154.0
134.80	182.0
137.00	167.0
140.90	1012.0
142.80	1405.0
144.90	631.0
145.80	204.0
147.90	260.0
154.90	357.0
156.80	168.0
160.80	136.0
171.00	248.0
171.80	1356.0
173.00	1220.0
173.90	101008.0
174.90	7756.0
175.90	97312.0
176.90	6568.0
178.00	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB169

m/z	Abundance
35.90	927.0
36.90	4626.0
37.90	4080.0
38.90	1913.0
39.80	184.0
44.00	728.0
44.90	754.0
46.10	168.0
47.00	1367.0
47.90	565.0
48.90	4605.0
49.90	21720.0
50.90	6385.0
52.00	318.0
55.00	256.0
55.90	1883.0
56.90	2826.0
57.90	129.0
59.90	1127.0
60.90	5149.0
61.90	5338.0
63.00	4869.0
63.90	872.0
64.90	1019.0
66.00	169.0
66.90	386.0
67.90	11589.0
68.90	12007.0
69.90	1012.0
71.90	659.0
72.90	5313.0
73.90	19632.0
74.90	59600.0
76.00	5807.0
77.00	776.0
77.90	598.0
78.90	4374.0
79.90	1256.0
80.80	4901.0
81.90	893.0
85.90	256.0
86.90	5642.0
87.90	5189.0
90.90	458.0
91.90	3773.0
93.00	5562.0
94.00	14750.0
95.00	123088.0
95.90	8423.0
96.90	199.0
103.90	527.0
104.90	159.0
105.80	716.0
113.00	103.0
114.70	160.0
115.80	507.0
116.90	906.0
117.80	576.0
118.80	636.0
127.80	369.0
128.80	214.0
129.90	483.0
130.80	198.0
134.80	229.0
137.00	165.0
140.90	1136.0
142.90	1568.0
144.90	606.0
145.80	203.0
147.90	306.0
153.60	107.0
154.90	288.0
156.80	171.0
158.90	107.0
160.80	159.0
171.00	264.0
171.80	1584.0
173.00	1354.0
173.90	108744.0
174.90	8275.0
175.90	105440.0
176.90	6945.0
178.00	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB169

m/z	Abundance
35.90	835.0
36.90	4144.0
37.90	3879.0
38.90	1793.0
39.80	176.0
44.00	800.0
44.80	799.0
46.10	131.0
47.00	1206.0
47.80	581.0
49.00	4175.0
50.00	20560.0
50.90	6026.0
52.00	293.0
52.90	103.0
55.00	255.0
56.00	1841.0
56.90	2798.0
57.90	106.0
59.90	1069.0
60.90	4837.0
62.00	4996.0
63.00	4794.0
63.90	801.0
64.90	982.0
66.00	125.0
66.90	354.0
67.90	11152.0
68.90	12003.0
69.90	828.0
71.90	657.0
72.90	5237.0
73.90	18656.0
74.90	57096.0
76.00	5158.0
77.00	776.0
77.90	582.0
78.80	4235.0
79.90	1238.0
80.80	4566.0
81.80	870.0
85.90	247.0
86.90	5545.0
87.90	4907.0
90.90	451.0
91.90	3592.0
93.00	5126.0
94.00	14223.0
95.00	119064.0
95.90	7641.0
96.90	185.0
103.90	516.0
104.90	173.0
105.80	668.0
112.00	155.0
114.70	176.0
115.80	470.0
116.90	929.0
117.80	548.0
118.80	713.0
123.80	109.0
127.80	422.0
128.80	232.0
129.80	448.0
130.90	199.0
134.80	246.0
136.90	128.0
140.90	1146.0
142.90	1611.0
144.90	499.0
145.80	194.0
147.90	304.0
152.70	113.0
154.90	262.0
156.80	170.0
158.90	116.0
160.90	185.0
171.00	283.0
171.80	1574.0
173.00	1295.0
173.90	107000.0
174.90	7812.0
175.90	103664.0
176.90	6614.0
177.90	264.0

Instrument :
MSVOA_U
ClientSampleId :
BFB169