


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070419\
 Data File : VU033165.D
 Acq On : 03 Jul 2019 11:50
 Operator : JC/SP
 Sample : BFB24
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jul 05 06:41:58 2019

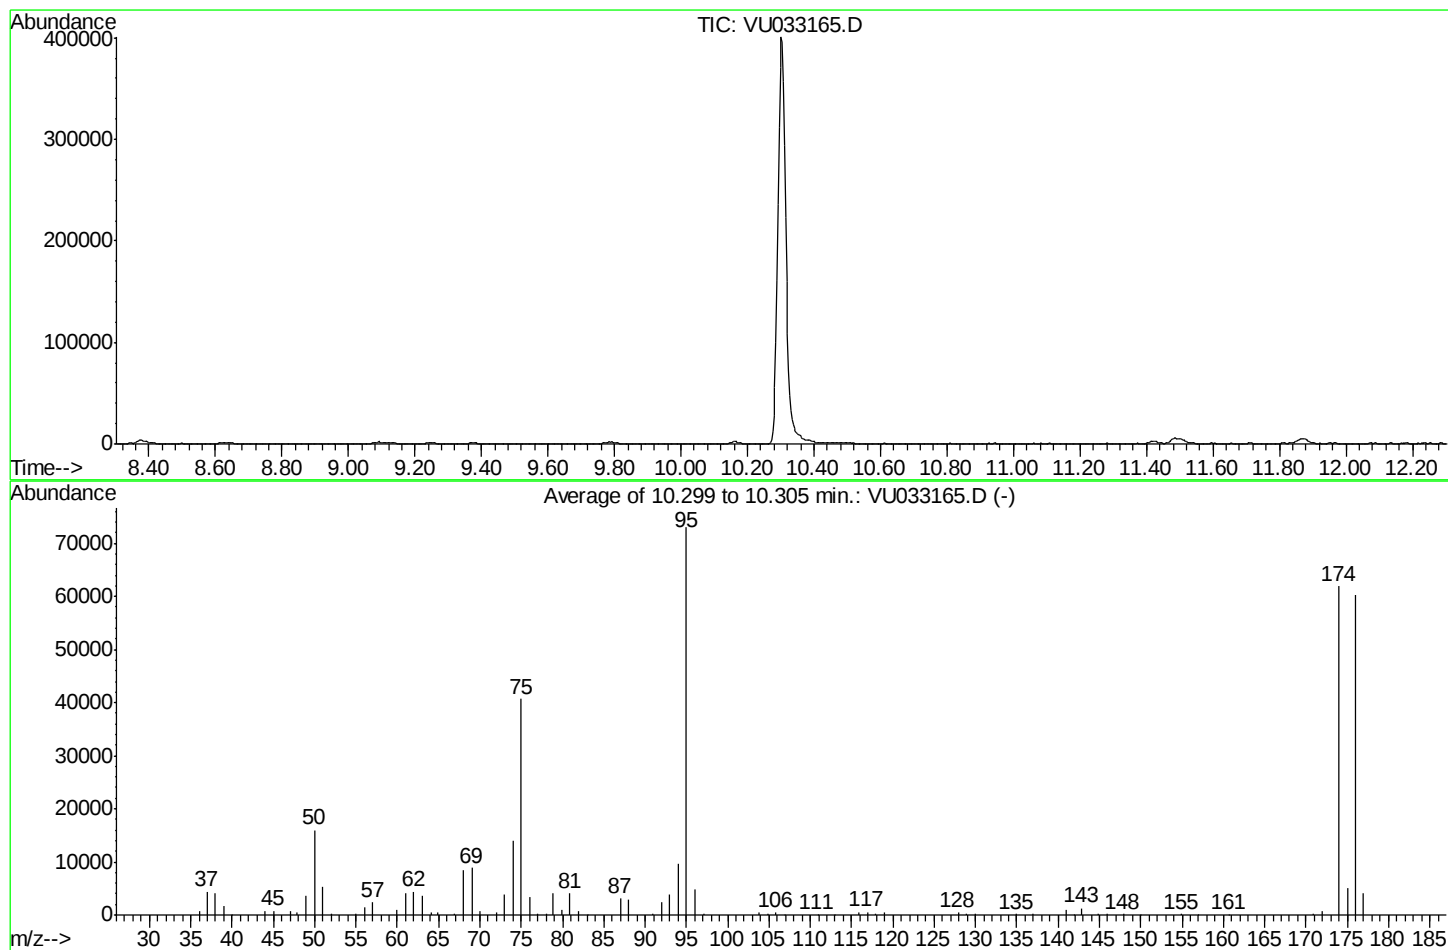

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	16036	PASS
75	95	30	80	55.7	40650	PASS
95	95	100	100	100.0	73013	PASS
96	95	5	9	6.7	4861	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	61925	PASS
175	174	5	9	8.3	5112	PASS
176	174	95	101	97.3	60282	PASS
177	176	5	9	6.8	4126	PASS

m/z	Abundance
44.00	321.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	784.0
37.00	4178.0
38.00	4100.0
39.00	1709.0
39.90	102.0
43.90	941.0
45.00	789.0
47.00	852.0
47.90	582.0
49.00	3452.0
50.00	15758.0
51.00	5206.0
52.00	243.0
55.00	261.0
56.00	1327.0
57.00	2453.0
60.00	926.0
61.00	3933.0
62.00	4257.0
63.00	3355.0
64.00	443.0
64.90	378.0
66.90	251.0
68.00	8163.0
69.00	8375.0
70.00	766.0
72.00	438.0
73.00	3748.0
74.00	13496.0
75.00	38696.0
76.00	3518.0
76.90	413.0
78.10	265.0
78.90	3758.0
79.90	911.0
80.90	3904.0
81.90	739.0
83.00	127.0
87.00	3090.0
88.00	2653.0
91.00	318.0
92.00	2283.0
93.00	3712.0
94.00	9406.0
95.00	69872.0
96.00	4696.0
97.10	109.0
103.90	423.0
104.90	174.0
105.90	466.0
106.90	104.0
115.80	316.0
116.90	572.0
117.90	254.0
118.90	567.0
127.90	310.0
128.90	153.0
129.90	319.0
135.00	169.0
137.10	138.0
141.00	861.0
142.90	1272.0
144.90	232.0
146.00	107.0
147.90	257.0
154.90	169.0
156.90	139.0
160.70	112.0
171.00	142.0
172.00	683.0
174.00	57624.0
175.00	4719.0
176.00	56736.0
177.00	3810.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	822.0
37.00	4434.0
38.00	4310.0
39.00	1762.0
39.90	109.0
43.90	1023.0
45.00	775.0
47.00	848.0
47.90	579.0
49.00	3718.0
50.00	16488.0
51.00	5583.0
52.00	290.0
55.00	245.0
56.00	1564.0
57.00	2468.0
60.00	935.0
61.00	4208.0
62.00	4577.0
63.00	3686.0
64.00	432.0
65.00	402.0
66.90	254.0
68.00	8739.0
69.00	9141.0
70.00	779.0
72.00	478.0
73.00	3880.0
74.00	14332.0
75.00	42016.0
76.00	3573.0
76.90	354.0
78.10	295.0
78.90	4179.0
79.90	918.0
80.90	4131.0
81.90	788.0
83.00	133.0
87.00	3255.0
88.00	2886.0
90.90	355.0
92.00	2409.0
93.00	4100.0
94.00	10012.0
95.00	75288.0
96.00	5025.0
97.00	157.0
103.80	432.0
104.80	142.0
105.90	500.0
106.90	117.0
113.00	127.0
115.80	376.0
116.90	622.0
117.90	306.0
118.90	534.0
127.90	423.0
128.90	183.0
129.90	318.0
135.00	215.0
137.00	148.0
140.90	978.0
141.80	113.0
142.90	1290.0
144.80	251.0
146.00	157.0
147.90	233.0
149.90	100.0
155.00	175.0
156.90	132.0
160.70	112.0
171.00	153.0
172.00	708.0
174.00	63624.0
175.00	5261.0
176.00	62160.0
177.00	4259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	841.0
37.00	4429.0
38.00	4044.0
39.00	1603.0
39.90	113.0
44.00	1042.0
45.00	707.0
47.00	814.0
47.90	584.0
49.00	3546.0
50.00	15863.0
51.00	5304.0
52.00	291.0
54.90	204.0
56.00	1544.0
57.00	2201.0
60.00	852.0
61.00	4191.0
62.00	4553.0
63.00	3674.0
64.10	383.0
65.00	453.0
67.00	238.0
68.00	8695.0
69.00	9058.0
70.00	730.0
71.90	525.0
73.00	3817.0
74.00	13877.0
75.00	41240.0
76.00	3329.0
77.00	337.0
78.10	303.0
78.90	4213.0
79.90	858.0
80.90	3976.0
81.90	763.0
83.00	135.0
87.00	3029.0
87.90	2896.0
90.90	375.0
92.00	2318.0
93.00	3984.0
94.00	9594.0
95.00	73880.0
96.00	4863.0
97.00	165.0
103.80	442.0
104.80	106.0
105.80	458.0
106.80	108.0
110.90	109.0
113.00	149.0
115.80	430.0
116.90	637.0
117.90	328.0
118.90	510.0
127.90	431.0
128.90	193.0
129.90	288.0
134.90	206.0
136.90	173.0
140.90	1035.0
141.90	145.0
142.90	1124.0
144.80	244.0
146.00	183.0
147.90	184.0
149.90	142.0
154.90	171.0
156.90	123.0
170.90	135.0
172.00	662.0
174.00	64528.0
175.00	5356.0
176.00	61952.0
177.00	4309.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24