

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070518\
 Data File : VU025207.D
 Acq On : 05 Jul 2018 11:45
 Operator : MD/SY
 Sample : J3783-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 S10-0148

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.088	137	155	175	rBV	436481	532870	25.57%	2.954%
2	1.404	246	253	262	rBV	38912	38994	1.87%	0.216%
3	1.757	354	363	383	rBV	236496	313131	15.02%	1.736%
4	2.310	523	535	551	rVB3	14464	33787	1.62%	0.187%
5	2.442	566	576	597	rVB	21585	37742	1.81%	0.209%
6	2.709	643	659	678	rBV	166318	354798	17.02%	1.967%
7	2.998	734	749	766	rBV	37544	78602	3.77%	0.436%
8	3.998	1041	1060	1079	rBV3	67073	183686	8.81%	1.018%
9	4.101	1079	1092	1106	rVV3	12851	35141	1.69%	0.195%
10	4.227	1108	1131	1152	rVB6	20338	74909	3.59%	0.415%
11	4.741	1275	1291	1306	rBV5	10045	27606	1.32%	0.153%
12	4.886	1319	1336	1353	rBV2	181996	414656	19.90%	2.298%
13	4.989	1353	1368	1384	rVV	284189	643370	30.87%	3.566%
14	5.085	1384	1398	1424	rVV3	94504	234670	11.26%	1.301%
15	5.262	1427	1453	1457	rVV7	16466	41601	2.00%	0.231%
16	5.313	1457	1469	1484	rVV	196475	420007	20.15%	2.328%
17	5.397	1485	1495	1506	rVV3	28317	63184	3.03%	0.350%
18	5.487	1507	1523	1527	rVV4	33794	78876	3.78%	0.437%
19	5.542	1527	1540	1558	rVV	281879	711949	34.16%	3.946%
20	5.625	1558	1566	1579	rVB7	10505	24010	1.15%	0.133%
21	5.889	1634	1648	1672	rBV	374372	750988	36.03%	4.163%
22	6.413	1793	1811	1824	rBV6	45924	129423	6.21%	0.717%
23	6.481	1824	1832	1841	rVV2	18845	33780	1.62%	0.187%
24	6.538	1841	1850	1858	rVV3	21698	40393	1.94%	0.224%
25	6.590	1858	1866	1878	rVB2	24392	45808	2.20%	0.254%
26	6.744	1900	1914	1928	rVB4	19781	41878	2.01%	0.232%
27	6.828	1928	1940	1953	rBV	12302	23882	1.15%	0.132%
28	6.931	1953	1972	1988	rBV	219979	476800	22.88%	2.643%
29	7.053	1993	2010	2024	rBV	389268	800218	38.39%	4.435%
30	7.297	2058	2086	2105	rBV	304710	620786	29.79%	3.441%
31	7.571	2148	2171	2201	rVB	704688	1300798	62.41%	7.210%
32	7.715	2201	2216	2230	rBV	41971	84365	4.05%	0.468%
33	7.921	2268	2280	2298	rVB	76039	140846	6.76%	0.781%
34	8.050	2302	2320	2331	rBV2	26716	50560	2.43%	0.280%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070518\
 Data File : VU025207.D
 Acq On : 05 Jul 2018 11:45
 Operator : MD/SY
 Sample : J3783-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 S10-0148

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Title : SW846 8260

35	8.169	2344	2357	2380	rVB3	59507	127490	6.12%	0.707%
36	8.313	2389	2402	2409	rBV2	17063	30573	1.47%	0.169%
37	8.368	2409	2419	2425	rBV	137969	242118	11.62%	1.342%
38	8.493	2448	2458	2467	rBV4	17596	29925	1.44%	0.166%
39	8.609	2484	2494	2504	rBV	24602	41530	1.99%	0.230%
40	8.783	2534	2548	2560	rBV2	10825	20965	1.01%	0.116%
41	8.950	2588	2600	2612	rBV	33372	56081	2.69%	0.311%
42	9.027	2612	2624	2634	rVV	130687	224449	10.77%	1.244%
43	9.095	2634	2645	2664	rVV	532329	897339	43.05%	4.974%
44	9.191	2666	2675	2682	rVV4	15983	29246	1.40%	0.162%
45	9.252	2683	2694	2718	rVV	1297256	2084179	100.00%	11.552%
46	9.381	2721	2734	2746	rVV	107786	192289	9.23%	1.066%
47	9.445	2746	2754	2766	rVB2	25718	40920	1.96%	0.227%
48	9.577	2781	2795	2804	rBV4	11904	20931	1.00%	0.116%
49	9.956	2903	2913	2927	rVB6	10937	20989	1.01%	0.116%
50	10.172	2968	2980	2989	rBV	260675	414574	19.89%	2.298%
51	10.223	2989	2996	3010	rVB	66979	110485	5.30%	0.612%
52	10.310	3011	3023	3038	rBV	535633	883130	42.37%	4.895%
53	10.593	3100	3111	3133	rVB	246669	438659	21.05%	2.431%
54	10.712	3134	3148	3156	rVV	52720	85238	4.09%	0.472%
55	10.776	3156	3168	3179	rVB	46103	74668	3.58%	0.414%
56	10.976	3220	3230	3249	rBV	56403	103000	4.94%	0.571%
57	11.152	3277	3285	3298	rVB2	13559	21137	1.01%	0.117%
58	11.329	3332	3340	3358	rVB	44161	79908	3.83%	0.443%
59	11.432	3358	3372	3379	rBV2	37000	60021	2.88%	0.333%
60	11.487	3379	3389	3406	rVV	632202	1028251	49.34%	5.699%
61	11.574	3406	3416	3426	rVB	29453	45077	2.16%	0.250%
62	11.693	3442	3453	3463	rVB2	15588	25290	1.21%	0.140%
63	11.770	3463	3477	3487	rBV2	138693	271563	13.03%	1.505%
64	11.876	3500	3510	3528	rVB5	53235	115598	5.55%	0.641%
65	11.985	3535	3544	3554	rVB2	29215	43573	2.09%	0.242%
66	12.059	3554	3567	3581	rVB	73107	125309	6.01%	0.695%
67	12.149	3581	3595	3602	rBV	15924	25527	1.22%	0.141%
68	12.255	3619	3628	3633	rBV	27170	39907	1.91%	0.221%
69	12.291	3633	3639	3651	rVV	31318	54136	2.60%	0.300%
70	12.358	3651	3660	3682	rVV3	68879	161108	7.73%	0.893%
71	12.545	3711	3718	3728	rVB5	13822	22007	1.06%	0.122%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070518\
Data File : VU025207.D
Acq On : 05 Jul 2018 11:45
Operator : MD/SY
Sample : J3783-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
S10-0148

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Title : SW846 8260

72	12.654	3738	3752	3759	rBV	28532	53011	2.54%	0.294%
73	12.789	3780	3794	3801	rBV	10321	22110	1.06%	0.123%
74	13.123	3886	3898	3908	rBV3	155060	248882	11.94%	1.379%
75	13.291	3939	3950	3961	rVB	70080	111788	5.36%	0.620%
76	13.583	4029	4041	4046	rVV7	9966	21248	1.02%	0.118%
77	13.612	4046	4050	4068	rVB7	10932	23170	1.11%	0.128%
78	13.747	4080	4092	4117	rBV	231866	389985	18.71%	2.162%


Sum of corrected areas: 18041498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070518\
Data File : VU025207.D
Acq On : 05 Jul 2018 11:45
Operator : MD/SY
Sample : J3783-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
S10-0148

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

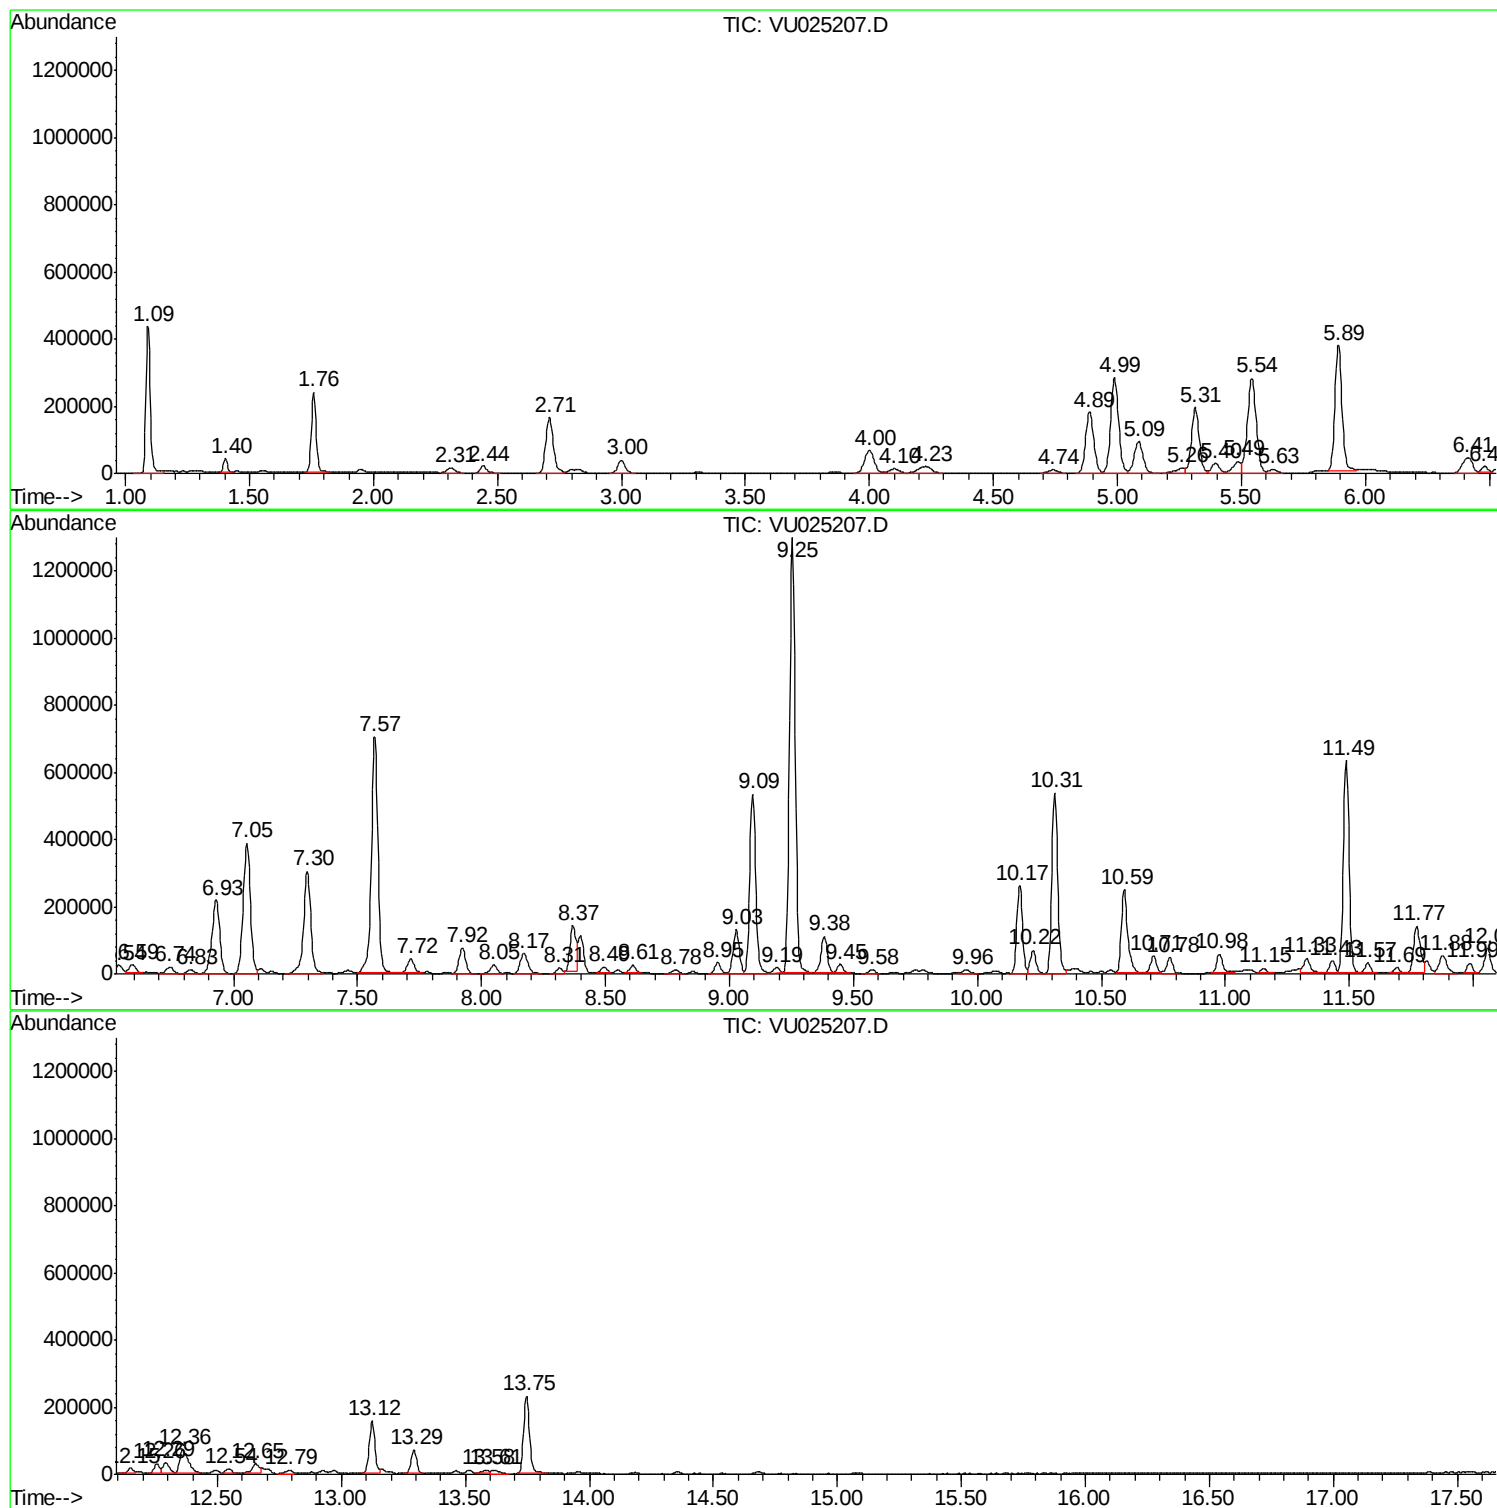

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070518\
Data File : VU025207.D
Acq On : 05 Jul 2018 11:45
Operator : MD/SY
Sample : J3783-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
S10-0148

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070518\
Data File : VU025207.D
Acq On : 05 Jul 2018 11:45
Operator : MD/SY
Sample : J3783-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
S10-0148

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc