


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070518\
 Data File : VU025203.D
 Acq On : 05 Jul 2018 09:34
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Title : SW846 8260
 Last Update : Wed Jun 13 13:55:26 2018

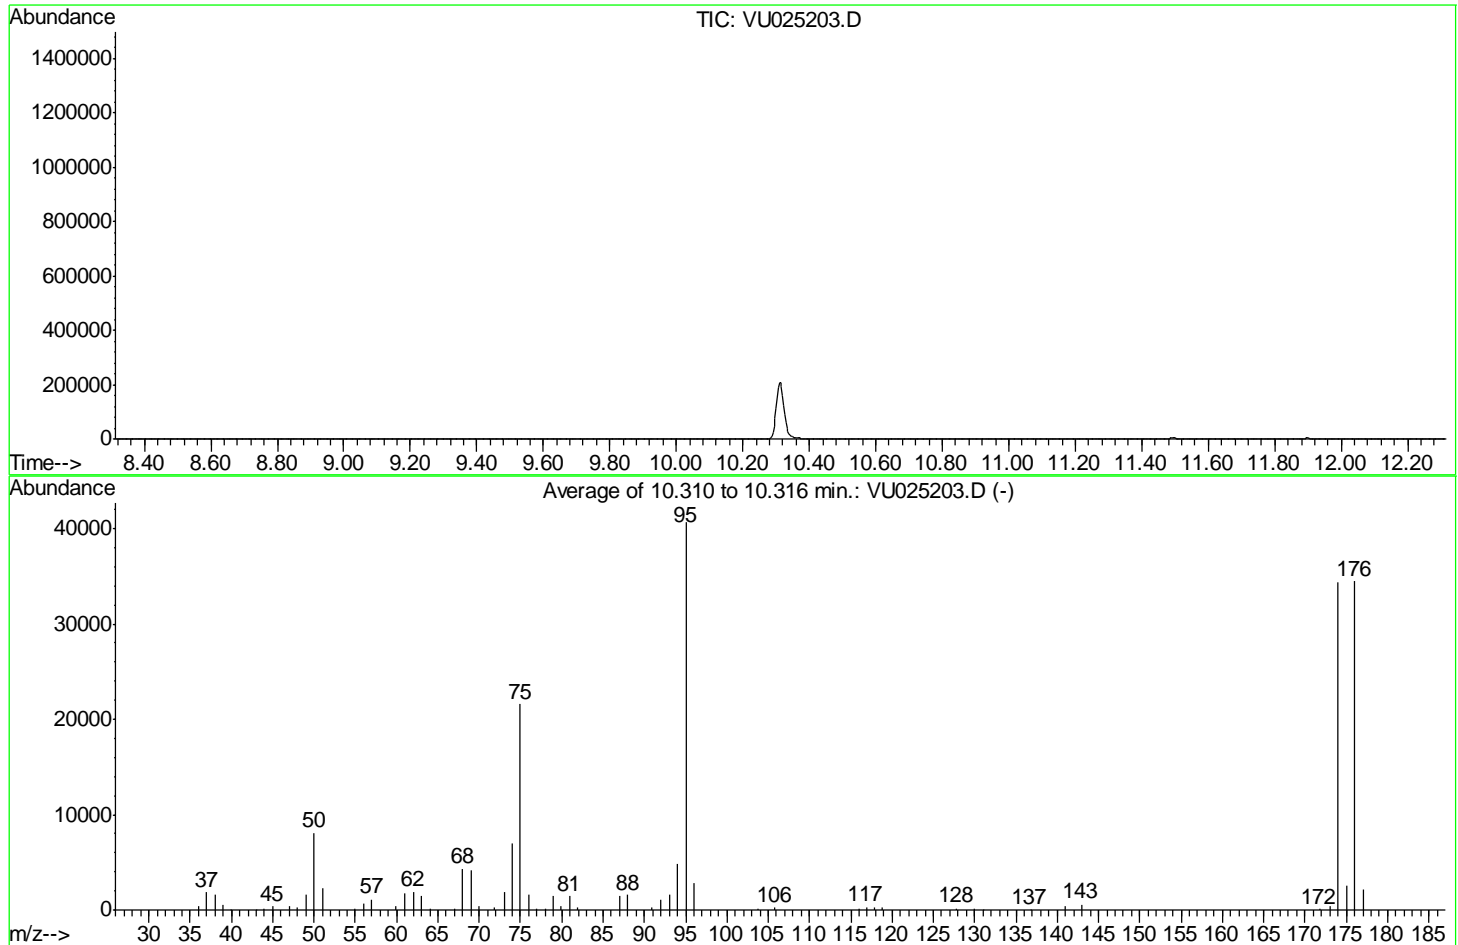

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8056	PASS
75	95	30	60	53.1	21581	PASS
95	95	100	100	100.0	40661	PASS
96	95	5	9	7.0	2835	PASS
173	174	0.00	2	1.3	450	PASS
174	95	50	100	84.7	34421	PASS
175	174	5	9	7.3	2520	PASS
176	174	95	101	100.1	34450	PASS
177	176	5	9	6.3	2182	PASS