


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070522\
Data File : VU049606.D
Acq On : 05 Jul 2022 08:55
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Title : SW846 8260
Last Update : Tue Jun 28 10:35:43 2022

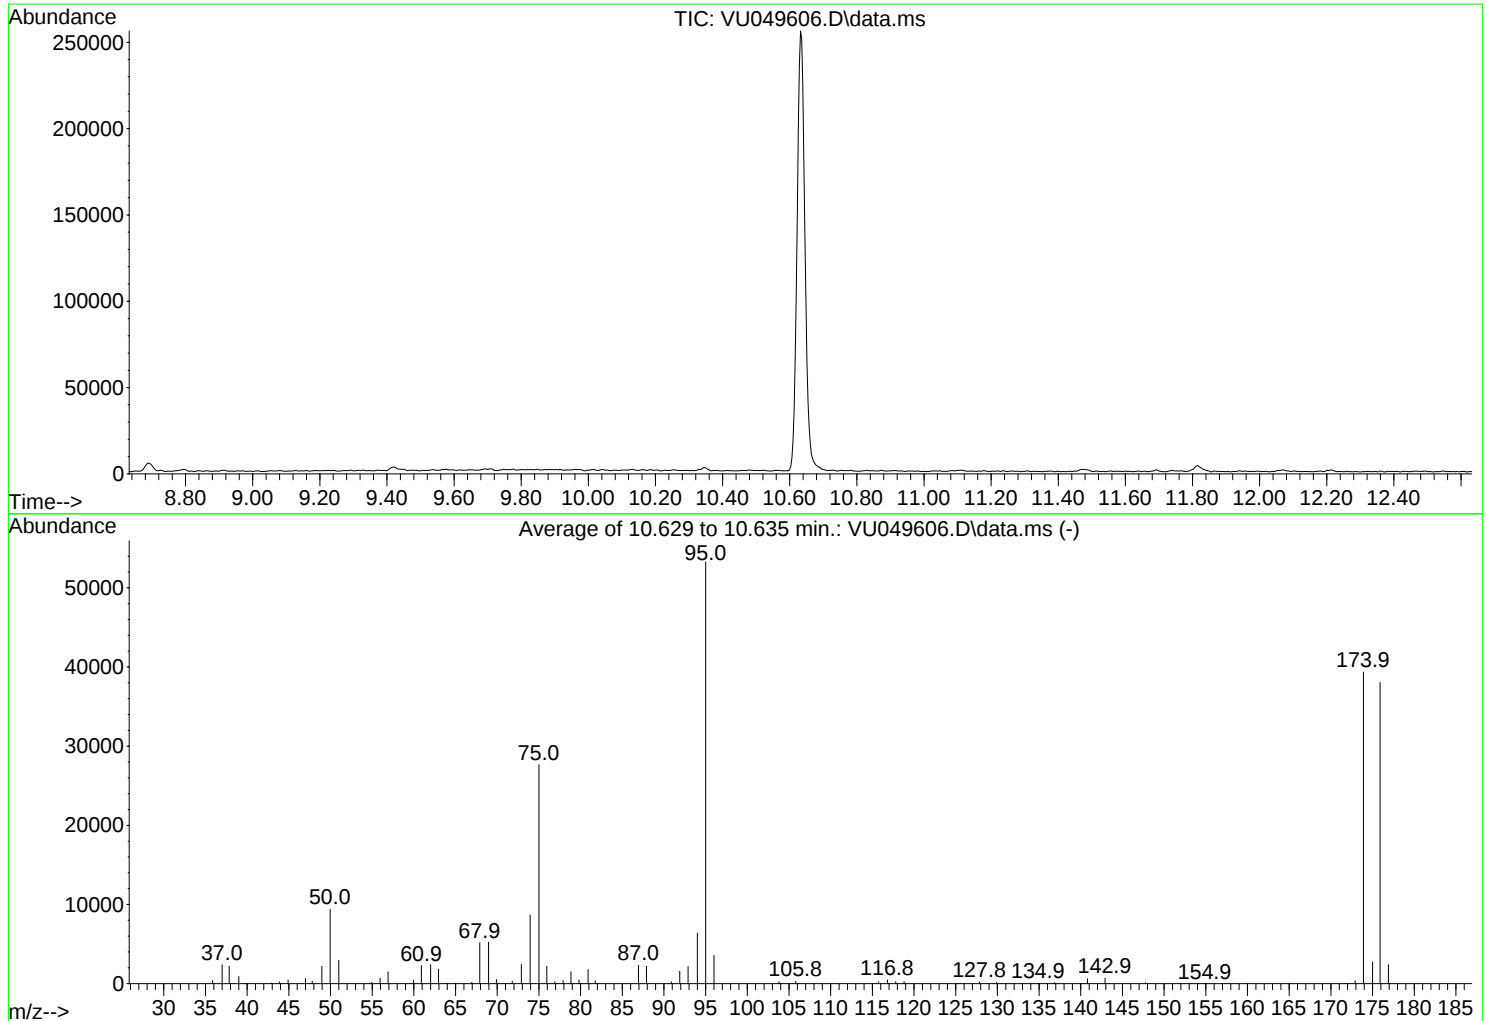

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	9384	PASS
75	95	30	60	51.9	27677	PASS
95	95	100	100	100.0	53288	PASS
96	95	5	9	6.7	3550	PASS
173	174	0.00	2	0.9	369	PASS
174	95	50	100	73.9	39387	PASS
175	174	5	9	6.9	2728	PASS
176	174	95	101	96.6	38040	PASS
177	176	5	9	6.3	2381	PASS