

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
 Data File : VU054765.D
 Acq On : 05 Jul 2023 12:44
 Operator : MD/SY
 Sample : 03495-14DL 4X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FC3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	34	rVB3	17550	23439	2.86%	0.322%
2	1.489	57	62	67	rBV2	12362	12603	1.54%	0.173%
3	1.596	87	95	112	rVB	71814	90998	11.12%	1.249%
4	1.907	185	192	206	rVB	63009	88471	10.81%	1.214%
5	2.560	383	395	412	rVB	113547	188147	22.99%	2.582%
6	2.792	456	467	475	rBV	5319	9757	1.19%	0.134%
7	3.039	534	544	559	rBV2	22452	42614	5.21%	0.585%
8	3.181	574	588	602	rBV	17614	39949	4.88%	0.548%
9	3.348	632	640	650	rBV2	6425	10913	1.33%	0.150%
10	4.660	1026	1048	1074	rBV2	229243	810226	98.99%	11.120%
11	5.058	1158	1172	1194	rVB	128419	290567	35.50%	3.988%
12	5.721	1357	1378	1398	rBV2	237366	633027	77.34%	8.688%
13	6.245	1528	1541	1565	rBV	263972	513110	62.69%	7.042%
14	6.538	1618	1632	1652	rBV	331950	634725	77.55%	8.711%
15	6.689	1666	1679	1697	rBV	159251	311082	38.01%	4.270%
16	7.563	1940	1951	1975	rBV2	79244	143346	17.51%	1.967%
17	7.894	2040	2054	2070	rBV	274691	477977	58.40%	6.560%
18	7.965	2070	2076	2092	rVB3	6521	12930	1.58%	0.177%
19	8.177	2131	2142	2161	rBV2	49878	86489	10.57%	1.187%
20	8.550	2245	2258	2272	rBV2	92789	161972	19.79%	2.223%
21	8.631	2272	2283	2325	rVV2	421877	818515	100.00%	11.234%
22	9.415	2514	2527	2543	rBV	371543	619984	75.74%	8.509%
23	10.753	2931	2943	2961	rBV	135191	220485	26.94%	3.026%
24	10.888	2976	2985	3000	rVB3	7159	11637	1.42%	0.160%
25	11.807	3260	3271	3292	rBV	352931	574014	70.13%	7.878%
26	12.190	3375	3390	3415	rBV	281791	459139	56.09%	6.302%




Sum of corrected areas: 7286116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
Data File : VU054765.D
Acq On : 05 Jul 2023 12:44
Operator : MD/SY
Sample : 03495-14DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

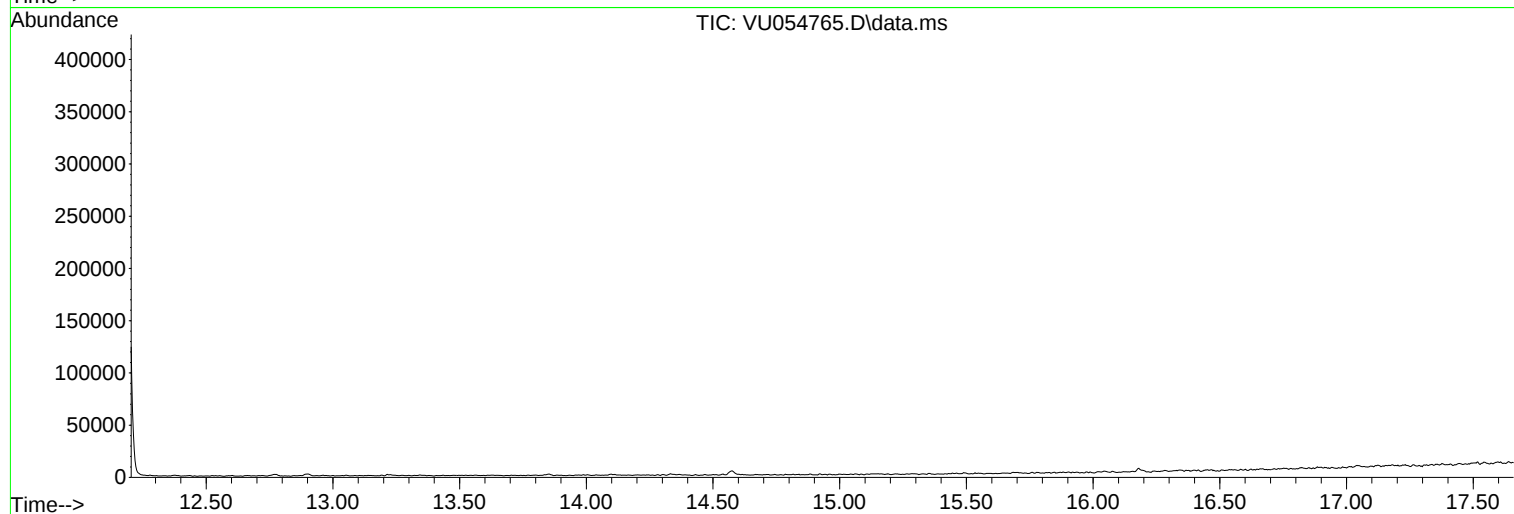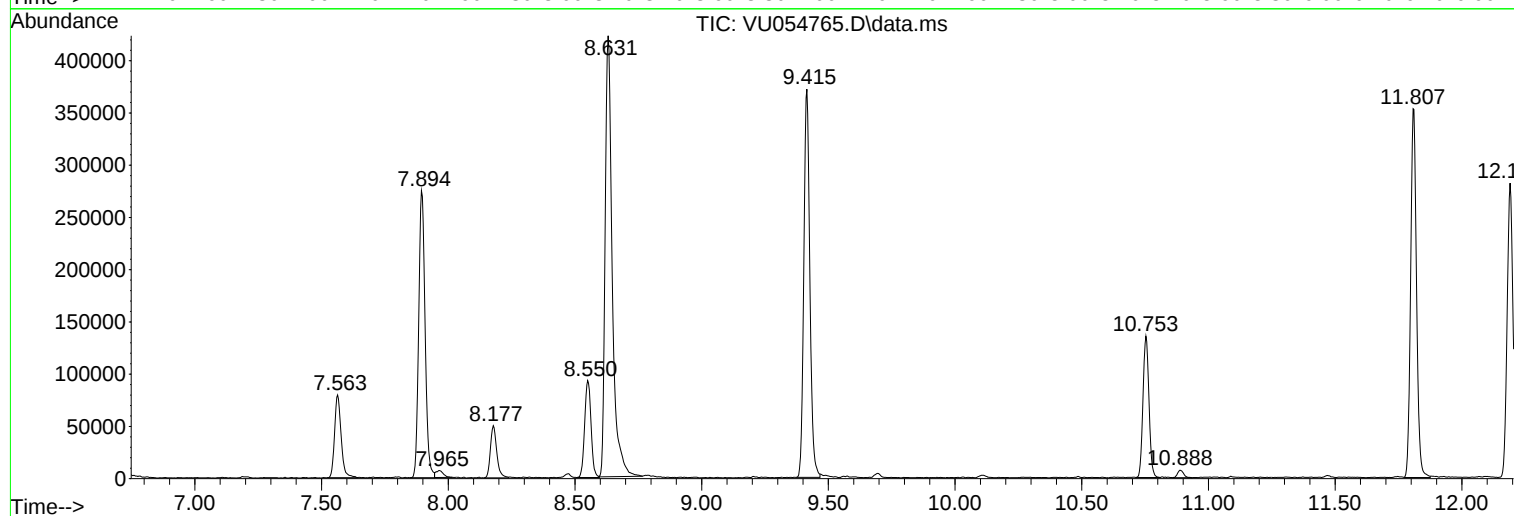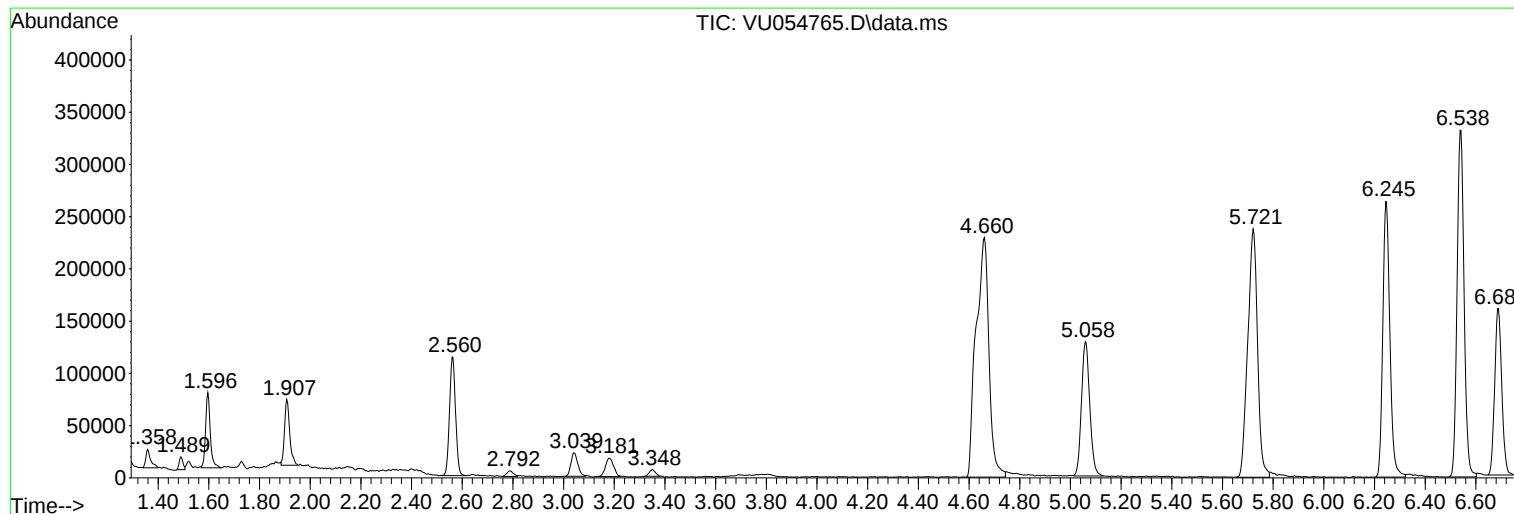

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
Data File : VU054765.D
Acq On : 05 Jul 2023 12:44
Operator : MD/SY
Sample : 03495-14DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
Data File : VU054765.D
Acq On : 05 Jul 2023 12:44
Operator : MD/SY
Sample : 03495-14DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc