

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
 Data File : VU054768.D
 Acq On : 05 Jul 2023 13:58
 Operator : MD/SY
 Sample : 03495-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	105	rBV	67465	79373	9.14%	1.308%
2	1.907	185	192	205	rVB	65717	92640	10.66%	1.527%
3	2.560	384	395	411	rVB	121725	198410	22.84%	3.270%
4	3.042	532	545	560	rBV2	24713	49133	5.66%	0.810%
5	4.624	1025	1037	1067	rBV	134141	353009	40.63%	5.818%
6	5.058	1156	1172	1195	rBV	132619	297489	34.24%	4.903%
7	5.721	1358	1378	1402	rBV3	249099	664091	76.44%	10.945%
8	6.245	1528	1541	1564	rBV	247677	474767	54.65%	7.825%
9	6.689	1665	1679	1698	rBV	169781	333502	38.39%	5.497%
10	7.563	1940	1951	1976	rBV	81487	148185	17.06%	2.442%
11	7.894	2041	2054	2071	rBV	282466	504799	58.10%	8.320%
12	8.177	2130	2142	2156	rBV	50202	89370	10.29%	1.473%
13	8.470	2220	2233	2244	rBV2	14595	23462	2.70%	0.387%
14	8.631	2271	2283	2318	rBV2	452413	868785	100.00%	14.319%
15	9.415	2513	2527	2549	rBV	350750	587165	67.58%	9.678%
16	10.753	2929	2943	2961	rBV	142567	233931	26.93%	3.856%
17	10.891	2973	2986	2998	rVB	25015	40964	4.72%	0.675%
18	11.811	3259	3272	3294	rBV	333571	541217	62.30%	8.920%
19	12.190	3378	3390	3416	rBV	292892	486960	56.05%	8.026%




Sum of corrected areas: 6067252

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
Data File : VU054768.D
Acq On : 05 Jul 2023 13:58
Operator : MD/SY
Sample : 03495-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

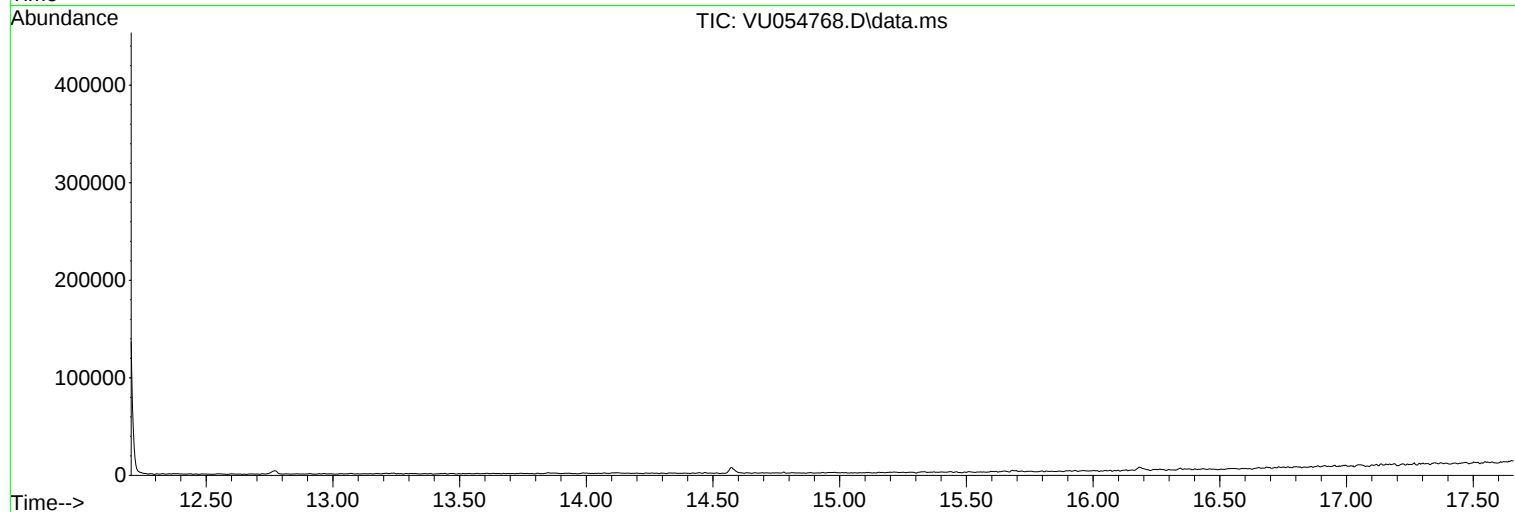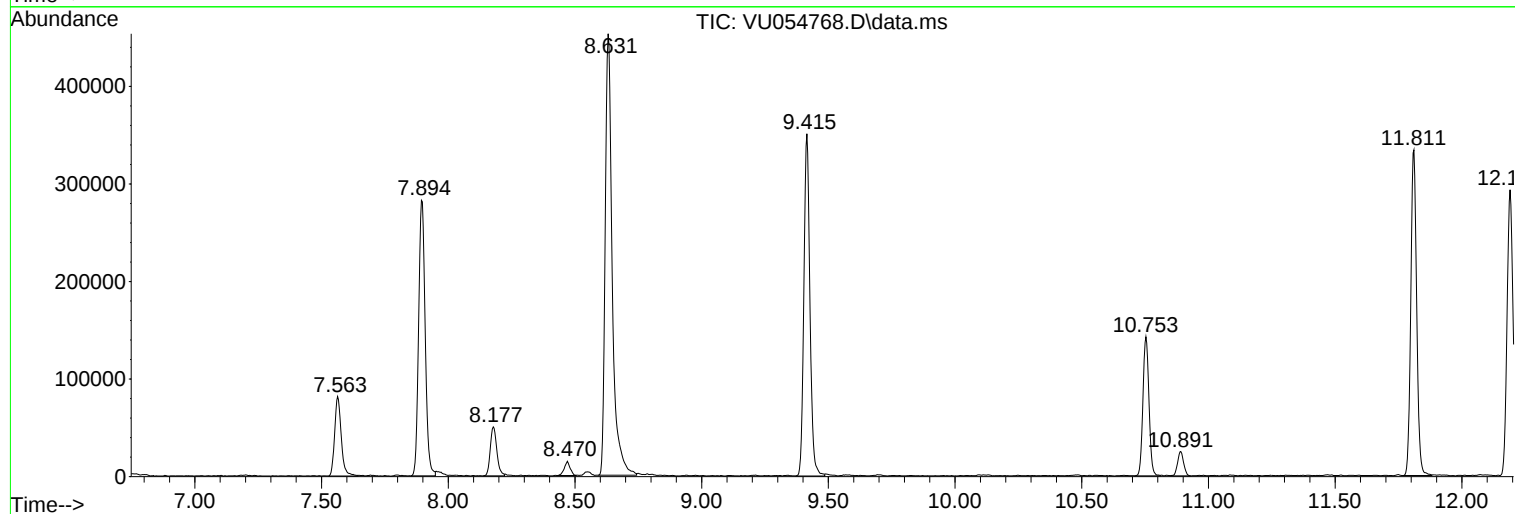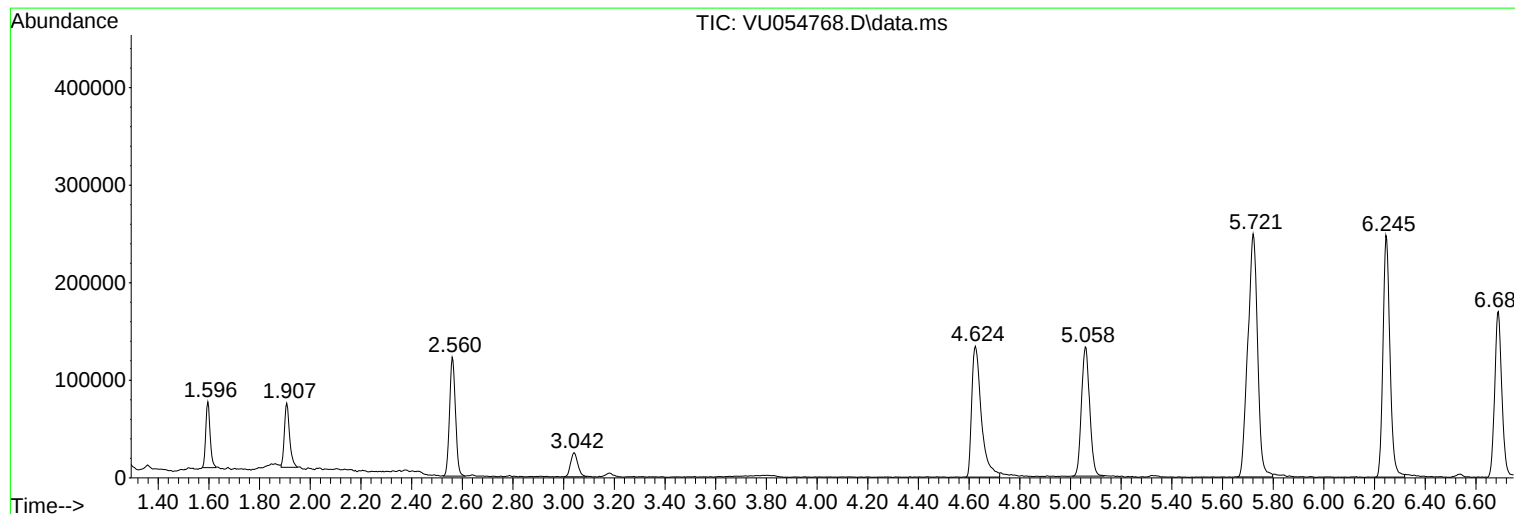

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
Data File : VU054768.D
Acq On : 05 Jul 2023 13:58
Operator : MD/SY
Sample : 03495-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
Data File : VU054768.D
Acq On : 05 Jul 2023 13:58
Operator : MD/SY
Sample : 03495-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc