


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070523\
Data File : VU054758.D
Acq On : 05 Jul 2023 08:49
Operator : MD/SY
Sample : BFB030
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB030

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jul 06 01:01:36 2023

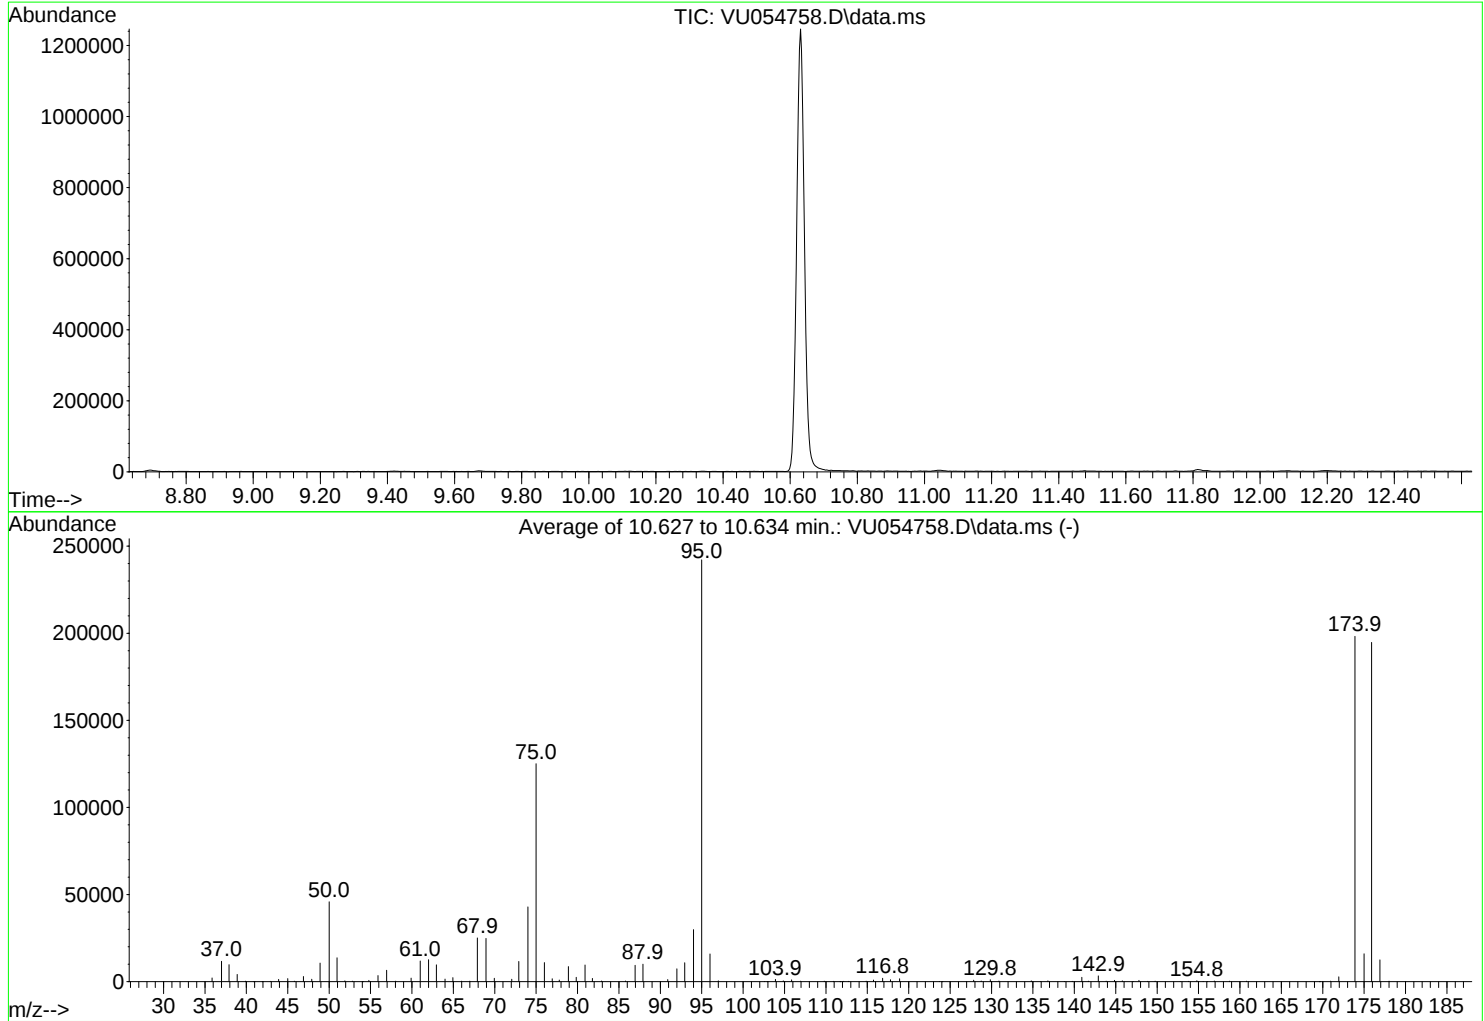

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	45832	PASS
75	95	30	80	51.7	125101	PASS
95	95	100	100	100.0	242155	PASS
96	95	5	9	6.6	15903	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.9	198272	PASS
175	174	5	9	8.1	16002	PASS
176	174	95	101	98.2	194752	PASS
177	176	5	9	6.4	12485	PASS

m/z	Abundance
35.80	411.0
37.80	158.0
39.80	124.0
44.00	446.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	2354.0
37.00	11601.0
38.00	9641.0
38.90	3943.0
40.00	429.0
40.90	104.0
41.90	156.0
42.90	177.0
43.90	1772.0
45.00	1783.0
45.80	376.0
46.90	3038.0
47.90	1301.0
48.90	10613.0
50.00	46256.0
51.00	14117.0
51.90	534.0
52.80	295.0
54.80	806.0
55.90	3401.0
57.00	6475.0
58.10	262.0
59.90	1871.0
61.00	12132.0
62.00	12516.0
62.90	9759.0
64.00	1472.0
64.90	2369.0
66.00	325.0
67.90	25192.0
69.00	24952.0
69.90	1800.0
72.10	1417.0
72.90	11670.0
74.00	42808.0
75.00	124048.0
76.00	11219.0
77.00	1528.0
77.80	853.0
78.90	8413.0
79.90	2319.0
80.90	9178.0
81.80	1874.0
82.90	417.0
85.90	423.0
87.00	8914.0
87.90	9863.0
90.90	1156.0
92.00	7309.0
92.90	10600.0
94.00	29776.0
95.00	239296.0
96.00	16416.0
97.10	426.0
102.60	127.0
102.90	122.0
103.90	1161.0
104.80	433.0
105.80	996.0
106.90	210.0
109.80	258.0
110.90	202.0
111.70	139.0
112.80	206.0
114.90	276.0
115.70	802.0
116.80	1838.0
117.80	921.0
118.90	1678.0
123.70	155.0
127.00	169.0
127.80	863.0
128.70	431.0
129.90	1060.0
130.90	315.0
134.70	530.0
135.90	108.0
136.80	471.0
138.80	165.0
139.70	198.0
140.90	2371.0
141.70	268.0
142.90	3454.0
143.80	214.0
144.80	712.0
145.80	401.0
147.80	711.0
148.80	201.0
149.80	267.0
152.80	141.0
153.80	149.0
154.80	558.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

155.50	107.0
156.10	102.0
156.90	363.0
158.70	323.0
160.80	302.0
171.00	303.0
171.90	2604.0
173.90	193472.0
175.00	15510.0
175.90	187776.0
176.90	12188.0
178.00	324.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	2645.0
37.00	12039.0
37.90	10328.0
38.90	4254.0
40.00	432.0
42.90	222.0
43.90	1845.0
45.00	1748.0
45.80	302.0
46.90	3076.0
47.90	1422.0
48.90	11059.0
50.00	47528.0
51.00	14085.0
51.90	433.0
52.80	305.0
54.80	773.0
55.90	3698.0
56.90	6786.0
58.00	270.0
59.90	2025.0
61.00	12209.0
62.00	13100.0
63.00	10151.0
64.00	1552.0
64.90	2412.0
66.00	295.0
67.90	25864.0
68.90	25640.0
70.00	1970.0
72.00	1468.0
72.90	11977.0
74.00	44232.0
75.00	128848.0
76.00	11358.0
76.90	1691.0
77.80	974.0
78.90	9000.0
79.90	2604.0
80.90	9887.0
81.80	1953.0
82.90	435.0
85.80	366.0
86.90	9671.0
87.90	10391.0
90.90	1258.0
92.00	7566.0
93.00	11199.0
94.00	30880.0
95.00	249920.0
96.00	16528.0
96.90	422.0
102.60	136.0
103.90	1331.0
104.90	445.0
105.90	1006.0
107.00	241.0
109.80	271.0
110.90	201.0
112.20	222.0
112.80	192.0
114.80	281.0
115.80	929.0
116.80	2018.0
117.80	1125.0
118.90	1678.0
123.70	106.0
126.90	120.0
127.80	865.0
128.80	410.0
129.80	1145.0
130.90	362.0
134.80	510.0
135.90	144.0
136.80	535.0
138.80	126.0
139.70	206.0
140.90	2587.0
141.70	322.0
142.90	3330.0
143.80	252.0
144.90	776.0
145.80	466.0
147.10	171.0
147.80	749.0
148.90	185.0
149.80	240.0
152.80	132.0
153.80	201.0
154.80	583.0
155.60	127.0
156.10	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

156.90	347.0
158.70	320.0
160.80	307.0
170.90	304.0
171.90	2853.0
173.90	204544.0
175.00	16640.0
175.90	201792.0
176.90	12859.0
178.00	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	2521.0
37.00	11388.0
37.90	9786.0
38.90	4176.0
39.90	366.0
42.90	216.0
43.90	1621.0
45.00	1597.0
45.80	226.0
46.90	2663.0
47.90	1531.0
48.90	10309.0
50.00	43712.0
50.90	12994.0
51.90	405.0
52.80	273.0
54.00	150.0
54.80	658.0
55.90	3422.0
56.90	6351.0
58.00	246.0
59.90	2128.0
61.00	11339.0
62.00	12261.0
63.00	9161.0
64.00	1378.0
65.00	2264.0
66.00	299.0
67.00	758.0
67.90	24216.0
69.00	23904.0
70.00	1963.0
72.00	1300.0
72.90	11150.0
74.00	41640.0
75.00	122408.0
76.00	10180.0
76.90	1698.0
77.80	1041.0
78.90	8369.0
79.80	2496.0
80.90	9513.0
81.80	1772.0
82.90	315.0
85.70	258.0
86.90	9679.0
87.90	9705.0
90.90	1216.0
92.00	7195.0
93.00	10817.0
94.00	28920.0
95.00	237248.0
96.00	14764.0
97.00	423.0
103.90	1332.0
104.90	406.0
105.90	1040.0
107.00	274.0
109.80	232.0
110.90	163.0
112.10	258.0
112.70	170.0
114.80	221.0
115.80	956.0
116.90	2045.0
117.80	1156.0
118.90	1499.0
124.00	136.0
127.90	829.0
128.80	396.0
129.80	1005.0
130.90	362.0
134.90	484.0
135.90	137.0
136.80	506.0
138.80	124.0
139.80	190.0
140.90	2538.0
141.70	326.0
142.90	3119.0
143.90	258.0
144.90	776.0
145.80	508.0
147.10	148.0
147.80	697.0
148.80	186.0
149.60	235.0
153.80	169.0
154.80	653.0
155.60	104.0
156.10	146.0
156.90	369.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

158.80	319.0
160.80	265.0
169.60	115.0
170.90	322.0
172.00	2898.0
173.90	196800.0
175.00	15857.0
175.90	194688.0
176.90	12407.0
178.00	304.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030