

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070618\
 Data File : VU025236.D
 Acq On : 06 Jul 2018 12:18
 Operator : MD/SY
 Sample : J3834-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.632	8	13	15	rBV	308	301	0.003%	0.003%
2	0.674	23	26	30	rBV2	154	121	0.001%	0.001%
3	0.703	30	35	37	rVV2	176	154	0.001%	0.002%
4	0.728	41	43	47	rVV	245	169	0.001%	0.002%
5	0.754	49	51	52	rVV	153	52	0.000%	0.001%
6	0.770	53	56	58	rVV2	292	185	0.002%	0.002%
7	0.796	62	64	69	rVB	255	161	0.001%	0.002%
8	0.838	75	77	78	rBV	178	77	0.001%	0.001%
9	0.863	81	85	89	rBV2	215	264	0.002%	0.003%
10	0.905	95	98	102	rVB2	233	169	0.001%	0.002%
11	0.924	102	104	106	rBV	81	49	0.000%	0.000%
12	0.982	119	122	123	rBV	247	121	0.001%	0.001%
13	1.024	133	135	137	rBV	147	88	0.001%	0.001%
14	1.088	137	155	176	rBV	1004007	1182529	100.00%	11.752%
15	1.400	245	252	263	rVB	128251	136598	11.55%	1.358%
16	1.677	331	338	353	rVB	97828	131374	11.11%	1.306%
17	2.275	513	524	537	rBV	247609	380937	32.21%	3.786%
18	2.555	606	611	613	rBV	502	360	0.003%	0.004%
19	2.619	625	631	638	rBV3	1017	1651	0.14%	0.016%
20	2.677	647	649	652	rBV3	400	252	0.002%	0.003%
21	2.706	652	658	664	rVB3	1031	1506	0.13%	0.015%
22	2.841	690	700	712	rBV2	1483	3133	0.26%	0.031%
23	2.985	742	745	746	rBV	191	88	0.001%	0.001%
24	3.159	796	799	804	rBV2	270	273	0.002%	0.003%
25	3.188	805	808	813	rVB2	228	201	0.002%	0.002%
26	3.352	855	859	860	rBV	285	166	0.001%	0.002%
27	3.391	868	871	872	rBV	197	140	0.001%	0.001%
28	3.439	883	886	889	rVB	282	163	0.001%	0.002%
29	3.564	923	925	927	rBV	152	47	0.000%	0.000%
30	3.619	938	942	944	rBV	219	132	0.001%	0.001%
31	3.728	973	976	981	rVB	290	174	0.001%	0.002%
32	3.799	996	998	999	rBV	187	55	0.000%	0.001%
33	3.850	1011	1014	1018	rVV	185	131	0.001%	0.001%
34	3.873	1018	1021	1024	rVV2	343	268	0.002%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070618\
 Data File : VU025236.D
 Acq On : 06 Jul 2018 12:18
 Operator : MD/SY
 Sample : J3834-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis

35	3.889	1024	1026	1028	rVB	247	105	0.01%	0.001%
36	3.973	1049	1052	1055	rBV2	218	131	0.01%	0.001%
37	3.989	1055	1057	1061	rBV	140	124	0.01%	0.001%
38	4.175	1101	1115	1146	rBV2	108934	289849	24.51%	2.881%
39	4.497	1206	1215	1216	rBV	472	556	0.05%	0.006%
40	4.580	1238	1241	1244	rBV2	361	199	0.02%	0.002%
41	4.651	1246	1263	1291	rVV	182889	461348	39.01%	4.585%
42	4.870	1329	1331	1332	rBV	303	129	0.01%	0.001%
43	4.889	1332	1337	1344	rVV3	1036	1312	0.11%	0.013%
44	4.915	1344	1345	1347	rVB	430	105	0.01%	0.001%
45	4.953	1355	1357	1358	rBV	365	156	0.01%	0.002%
46	4.979	1363	1365	1367	rBV2	428	255	0.02%	0.003%
47	5.046	1383	1386	1388	rBV	229	145	0.01%	0.001%
48	5.149	1415	1418	1422	rBV	125	88	0.01%	0.001%
49	5.169	1422	1424	1426	rBV	143	61	0.01%	0.001%
50	5.207	1428	1436	1441	rVB2	271	374	0.03%	0.004%
51	5.236	1441	1445	1447	rBV2	238	218	0.02%	0.002%
52	5.342	1453	1478	1502	rBV2	380986	1154480	97.63%	11.473%
53	5.628	1564	1567	1569	rBV2	361	271	0.02%	0.003%
54	5.661	1574	1577	1578	rBV2	244	161	0.01%	0.002%
55	5.696	1584	1588	1591	rVB2	329	273	0.02%	0.003%
56	5.718	1591	1595	1596	rBV	89	59	0.00%	0.001%
57	5.751	1596	1605	1612	rBV	438	847	0.07%	0.008%
58	5.889	1633	1648	1672	rBV	383429	754128	63.77%	7.495%
59	6.333	1772	1786	1813	rBV	261443	526005	44.48%	5.228%
60	6.503	1834	1839	1842	rVB2	488	473	0.04%	0.005%
61	6.532	1842	1848	1849	rBV	351	259	0.02%	0.003%
62	6.558	1854	1856	1857	rBV	272	105	0.01%	0.001%
63	6.657	1885	1887	1892	rVB	363	290	0.02%	0.003%
64	6.683	1893	1895	1898	rVV2	165	97	0.01%	0.001%
65	6.728	1908	1909	1912	rVB	330	139	0.01%	0.001%
66	6.757	1915	1918	1919	rBV	257	136	0.01%	0.001%
67	6.908	1963	1965	1970	rBV	223	182	0.02%	0.002%
68	6.940	1973	1975	1977	rVB	165	66	0.01%	0.001%
69	6.960	1977	1981	1983	rBV	195	139	0.01%	0.001%
70	7.008	1994	1996	1998	rBV	91	40	0.00%	0.000%
71	7.056	2009	2011	2015	rVB2	295	193	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070618\
 Data File : VU025236.D
 Acq On : 06 Jul 2018 12:18
 Operator : MD/SY
 Sample : J3834-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis

72	7.114	2027	2029	2032	rVB2	189	108	0.01%	0.001%
73	7.172	2044	2047	2050	rBV	212	118	0.01%	0.001%
74	7.230	2052	2065	2086	rBV	150677	267826	22.65%	2.662%
75	7.387	2111	2114	2115	rBV	407	222	0.02%	0.002%
76	7.513	2151	2153	2155	rBV	127	74	0.01%	0.001%
77	7.567	2157	2170	2191	rBV	536411	936728	79.21%	9.309%
78	7.767	2229	2232	2234	rBV	203	147	0.01%	0.001%
79	7.805	2241	2244	2246	rBV2	188	119	0.01%	0.001%
80	7.853	2247	2259	2275	rBV	105158	177833	15.04%	1.767%
81	8.043	2317	2318	2319	rBV	107	32	0.00%	0.000%
82	8.082	2329	2330	2335	rBV	247	156	0.01%	0.002%
83	8.181	2350	2361	2362	rBV	744	904	0.08%	0.009%
84	8.233	2370	2377	2384	rBV5	1887	2485	0.21%	0.025%
85	8.313	2390	2402	2430	rBV	352440	620684	52.49%	6.168%
86	8.490	2455	2457	2459	rBV3	378	225	0.02%	0.002%
87	8.567	2478	2481	2485	rBV	311	190	0.02%	0.002%
88	8.921	2587	2591	2594	rBV2	202	162	0.01%	0.002%
89	8.979	2606	2609	2611	rBV2	205	114	0.01%	0.001%
90	8.992	2611	2613	2619	rBV	312	236	0.02%	0.002%
91	9.091	2631	2644	2681	rBV	518006	860176	72.74%	8.549%
92	9.255	2692	2695	2699	rBV3	504	443	0.04%	0.004%
93	9.673	2822	2825	2829	rBV2	229	197	0.02%	0.002%
94	9.895	2891	2894	2895	rBV2	284	181	0.02%	0.002%
95	10.152	2971	2974	2978	rBV2	345	292	0.02%	0.003%
96	10.201	2986	2989	2992	rBV2	365	347	0.03%	0.003%
97	10.435	3050	3062	3083	rBV	370340	591099	49.99%	5.874%
98	11.323	3336	3338	3340	rBV	324	202	0.02%	0.002%
99	11.487	3377	3389	3412	rBV	463665	748326	63.28%	7.437%
100	11.863	3494	3506	3531	rBV	502026	817053	69.09%	8.120%


Sum of corrected areas: 10062266

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU070618\
Data File : VU025236.D
Acq On : 06 Jul 2018 12:18
Operator : MD/SY
Sample : J3834-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

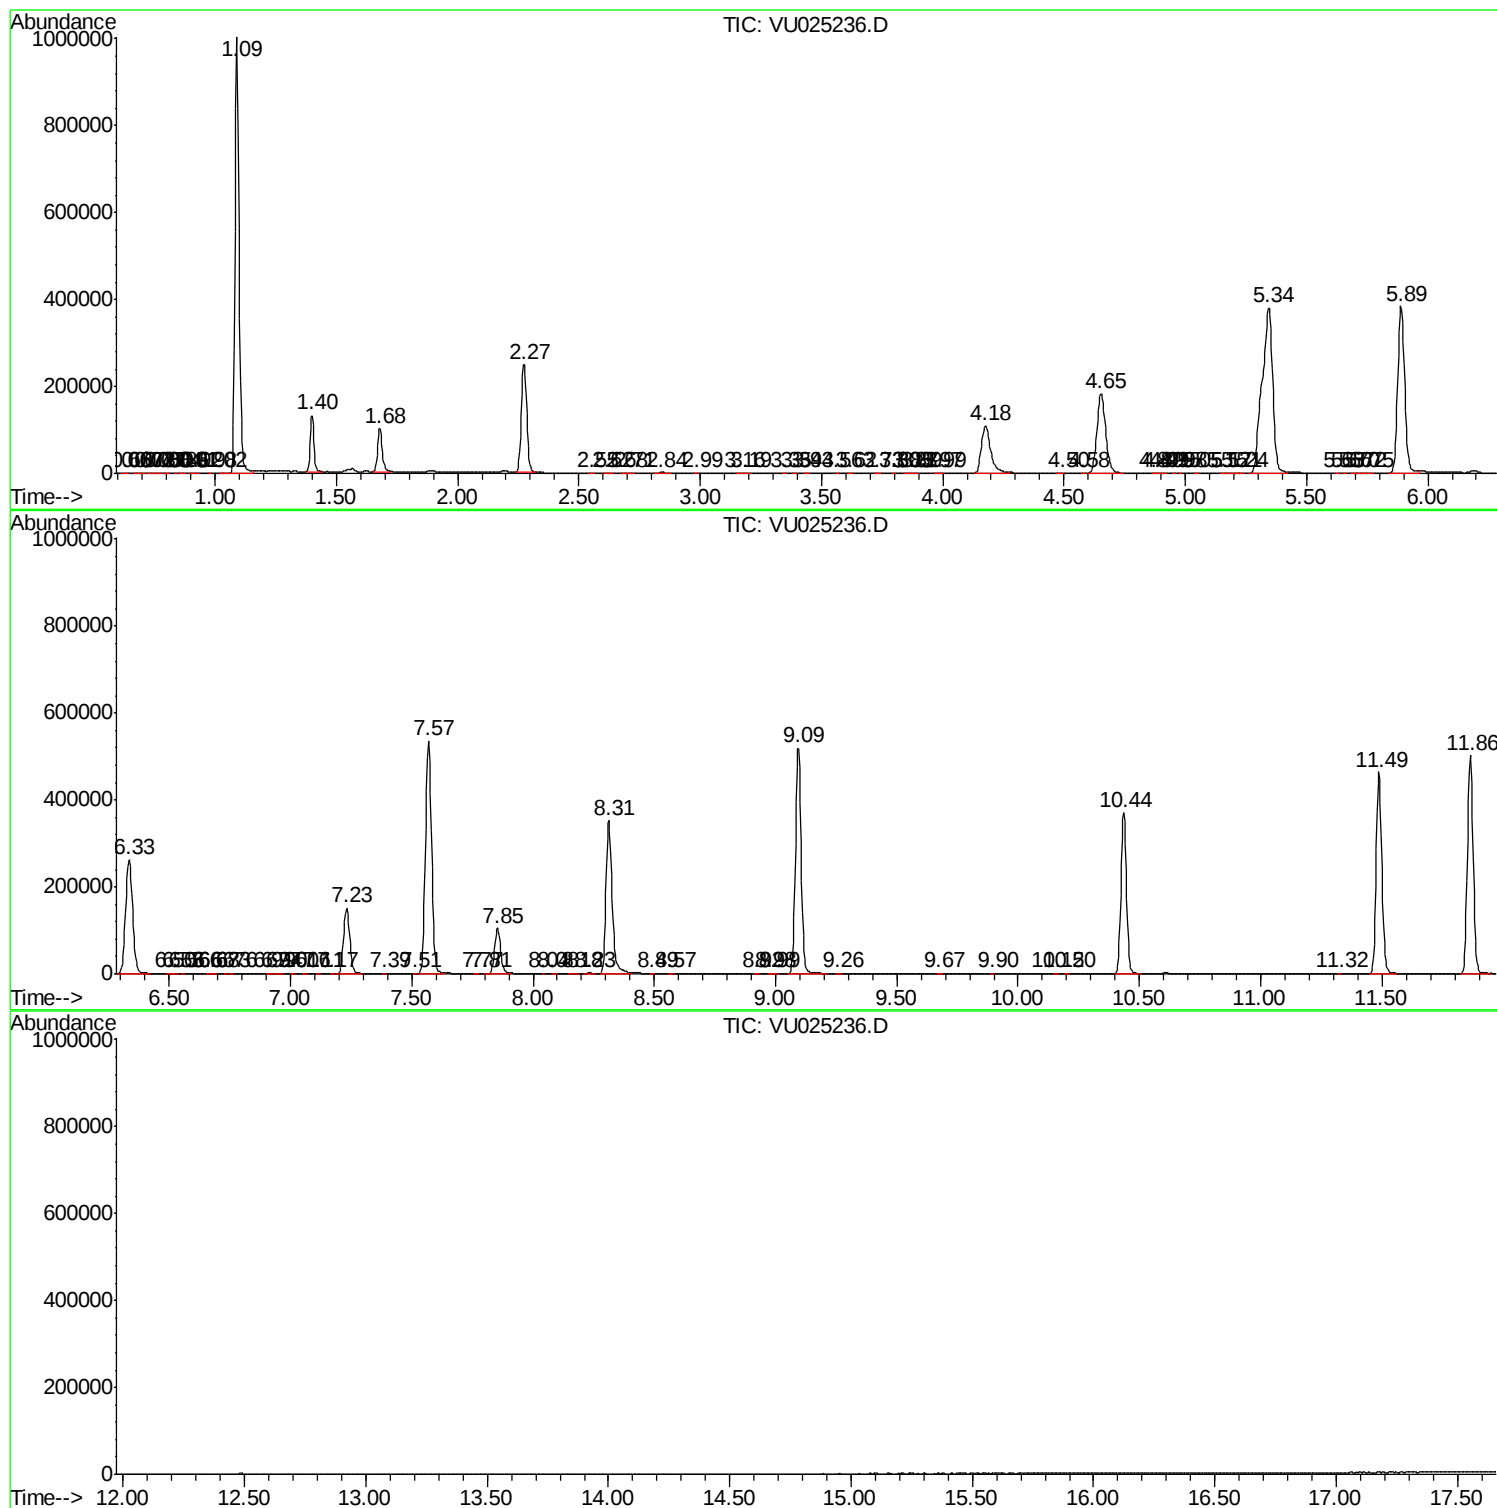

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU070618\
Data File : VU025236.D
Acq On : 06 Jul 2018 12:18
Operator : MD/SY
Sample : J3834-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU070618\
Data File : VU025236.D
Acq On : 06 Jul 2018 12:18
Operator : MD/SY
Sample : J3834-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc