


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070618\
 Data File : VU025231.D
 Acq On : 06 Jul 2018 09:01
 Operator : MD/SY
 Sample : BFB41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 06 23:15:38 2018

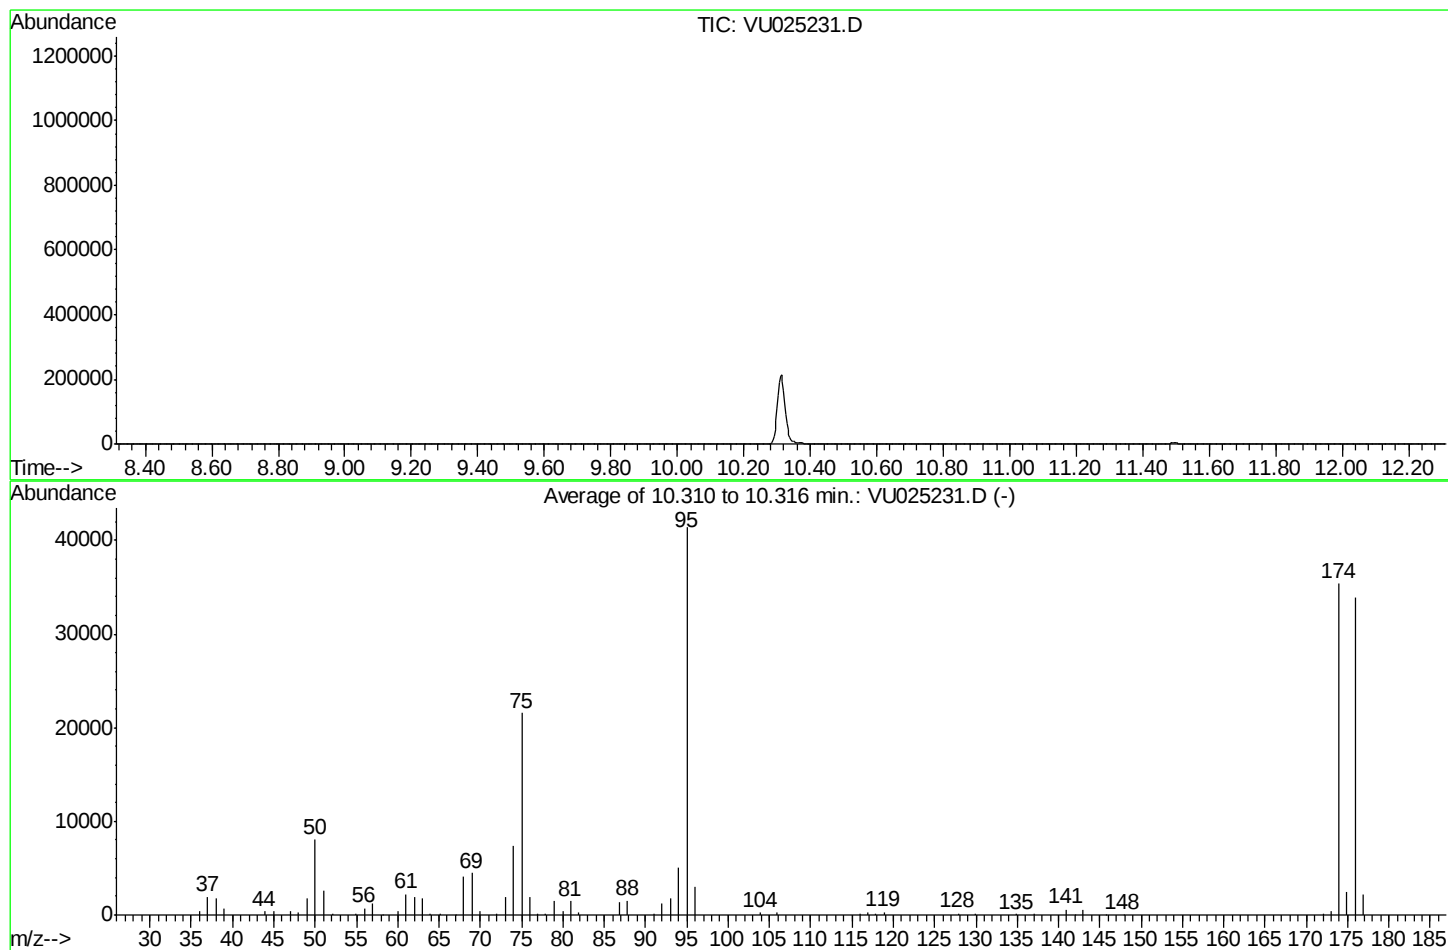

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	8000	PASS
75	95	30	80	52.1	21570	PASS
95	95	100	100	100.0	41389	PASS
96	95	5	9	7.2	2966	PASS
173	174	0.00	2	1.0	367	PASS
174	95	50	120	85.4	35336	PASS
175	174	5	9	7.0	2467	PASS
176	174	95	101	95.8	33848	PASS
177	176	5	9	6.7	2258	PASS

Scan 3011 (10.271 min): VU025231.D
BFB41

m/z	Abundance
40.00	112.0
43.90	395.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	494.0
37.00	1971.0
38.00	1853.0
39.00	736.0
43.90	859.0
45.00	375.0
47.00	422.0
47.90	272.0
49.00	1986.0
50.00	8286.0
51.00	2731.0
55.00	180.0
55.90	691.0
57.00	1379.0
60.00	481.0
61.00	2313.0
62.00	2092.0
63.00	1808.0
63.90	177.0
65.20	133.0
67.00	101.0
68.00	4377.0
69.00	4536.0
69.90	320.0
71.90	220.0
73.00	2107.0
74.00	7650.0
75.00	22472.0
76.00	2020.0
76.90	247.0
78.00	142.0
78.90	1454.0
80.00	458.0
80.90	1514.0
81.90	328.0
86.90	1476.0
87.90	1594.0
91.00	200.0
92.00	1300.0
93.00	1731.0
94.00	5184.0
95.00	42472.0
96.00	3208.0
103.90	196.0
105.90	258.0
116.00	121.0
116.90	249.0
117.90	219.0
118.80	325.0
127.90	194.0
129.90	201.0
134.90	132.0
137.00	104.0
140.90	516.0
142.90	552.0
147.90	108.0
172.00	121.0
173.00	366.0
174.00	35136.0
174.90	2471.0
176.00	33696.0
177.00	2235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	383.0
37.00	2016.0
38.00	1782.0
39.00	691.0
43.90	777.0
45.00	406.0
47.00	361.0
47.90	269.0
49.00	1848.0
50.00	8197.0
51.10	2780.0
52.10	101.0
54.90	200.0
56.00	736.0
57.00	1297.0
58.20	101.0
60.00	489.0
61.00	2294.0
62.00	2049.0
63.00	1819.0
63.90	144.0
65.20	125.0
68.00	4230.0
69.00	4624.0
69.90	397.0
71.90	191.0
73.00	2009.0
74.00	7635.0
75.00	22184.0
76.00	1948.0
76.90	175.0
77.80	130.0
78.90	1502.0
80.00	426.0
80.90	1513.0
81.90	322.0
86.90	1489.0
87.90	1556.0
91.00	201.0
92.00	1292.0
93.00	1801.0
94.00	5290.0
95.00	42584.0
96.00	3079.0
103.90	256.0
105.90	223.0
115.90	110.0
116.80	279.0
117.80	189.0
118.90	338.0
127.90	199.0
129.90	178.0
134.90	102.0
137.00	130.0
141.00	566.0
142.90	571.0
145.70	106.0
147.80	106.0
172.00	103.0
173.00	376.0
174.00	36528.0
174.90	2564.0
176.00	34928.0
177.00	2321.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	304.0
37.00	1798.0
38.00	1589.0
39.00	647.0
43.90	725.0
45.00	382.0
47.10	310.0
47.90	261.0
49.00	1548.0
50.00	7519.0
51.00	2356.0
52.10	144.0
54.90	226.0
56.00	646.0
57.00	1158.0
60.00	369.0
61.00	2100.0
62.00	1800.0
63.00	1591.0
64.00	106.0
67.00	115.0
68.00	3850.0
69.00	4221.0
69.90	436.0
71.90	174.0
73.00	1671.0
74.00	6873.0
75.00	20056.0
76.00	1649.0
76.80	131.0
77.80	116.0
78.90	1402.0
80.00	378.0
80.90	1352.0
81.90	279.0
86.90	1320.0
87.80	1394.0
91.00	148.0
92.00	1108.0
93.00	1664.0
94.00	4780.0
95.00	39112.0
96.00	2611.0
103.90	247.0
105.90	177.0
115.80	112.0
116.80	281.0
117.80	174.0
118.90	317.0
127.90	137.0
129.90	146.0
137.00	103.0
141.00	570.0
142.00	103.0
142.90	505.0
173.00	361.0
174.00	34344.0
174.90	2366.0
176.00	32920.0
176.90	2220.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41