

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070620\
 Data File : VU039288.D
 Acq On : 06 Jul 2020 14:05
 Operator : SY/MD
 Sample : L3193-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4296

Manual Integrations
 APPROVED

MMDadoda
 7/8/2020 2:52:44 PM

Quant Time: Jul 07 01:18:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:17:04 2020
 Response via : Initial Calibration

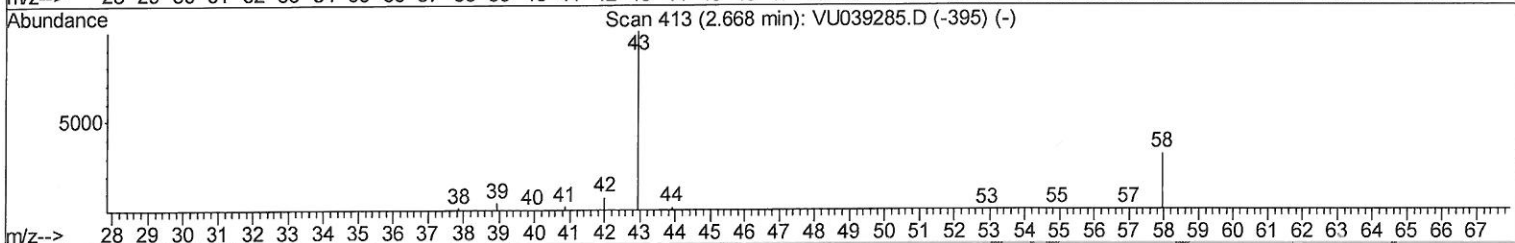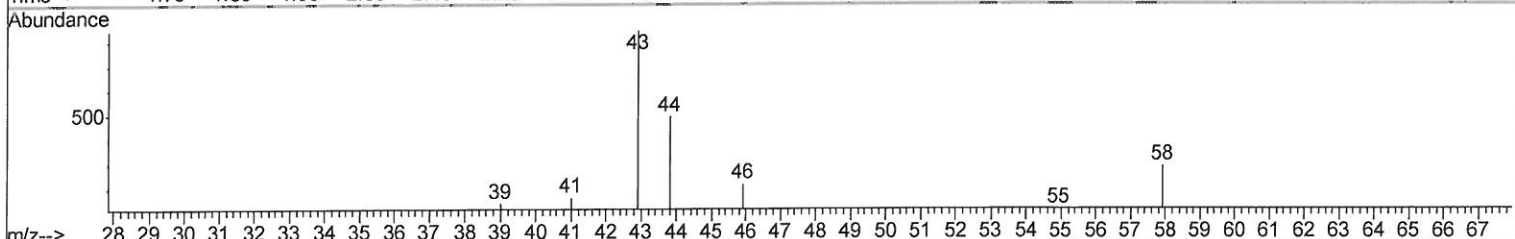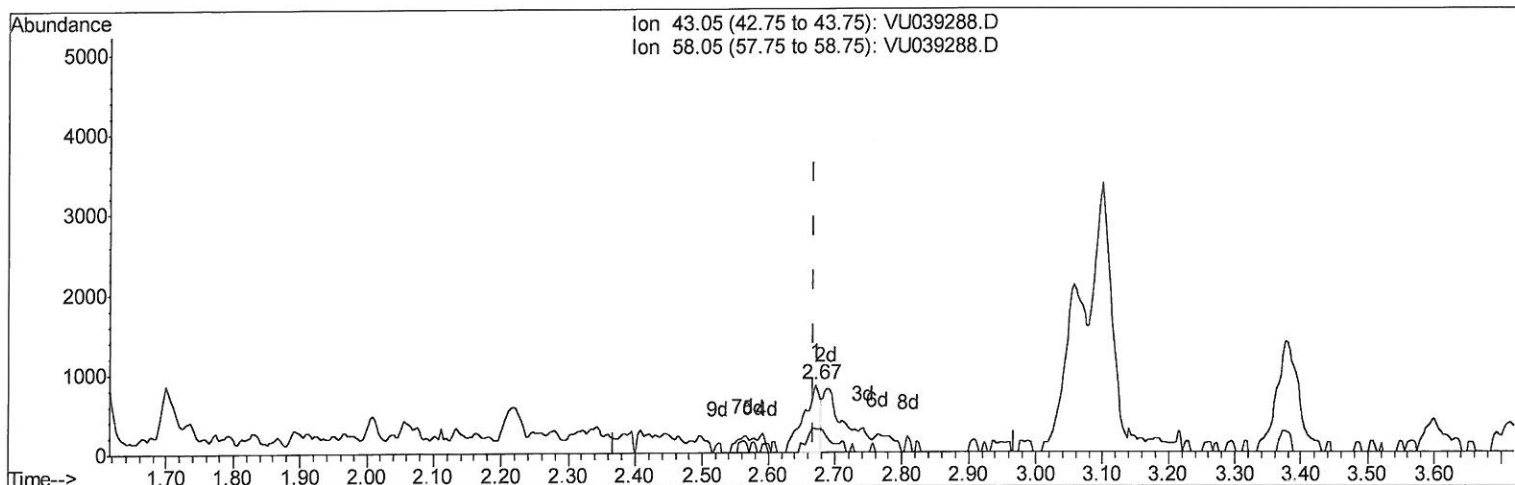

TIC: VU039288.D

(13) Acetone (T)

2.671min (+0.003) 0.85ug/L

response 1434

Ion	Exp%	Act%
43.05	100	100
58.05	31.80	46.79
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070620\
 Data File : VU039288.D
 Acq On : 06 Jul 2020 14:05
 Operator : SY/MD
 Sample : L3193-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4296

Manual Integrations
 APPROVED

MMDadoda
 7/8/2020 2:52:44 PM

Quant Time: Jul 07 01:18:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:17:04 2020
 Response via : Initial Calibration

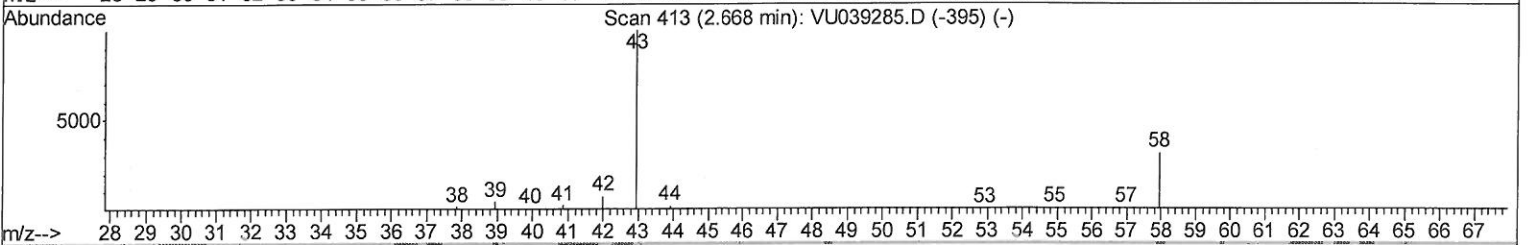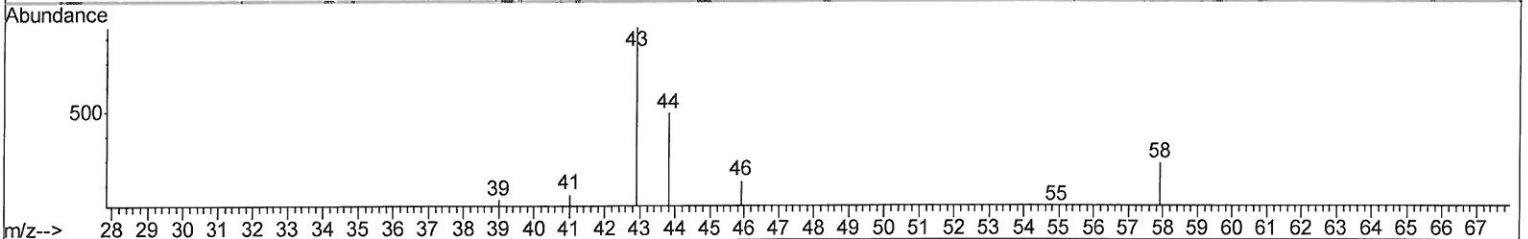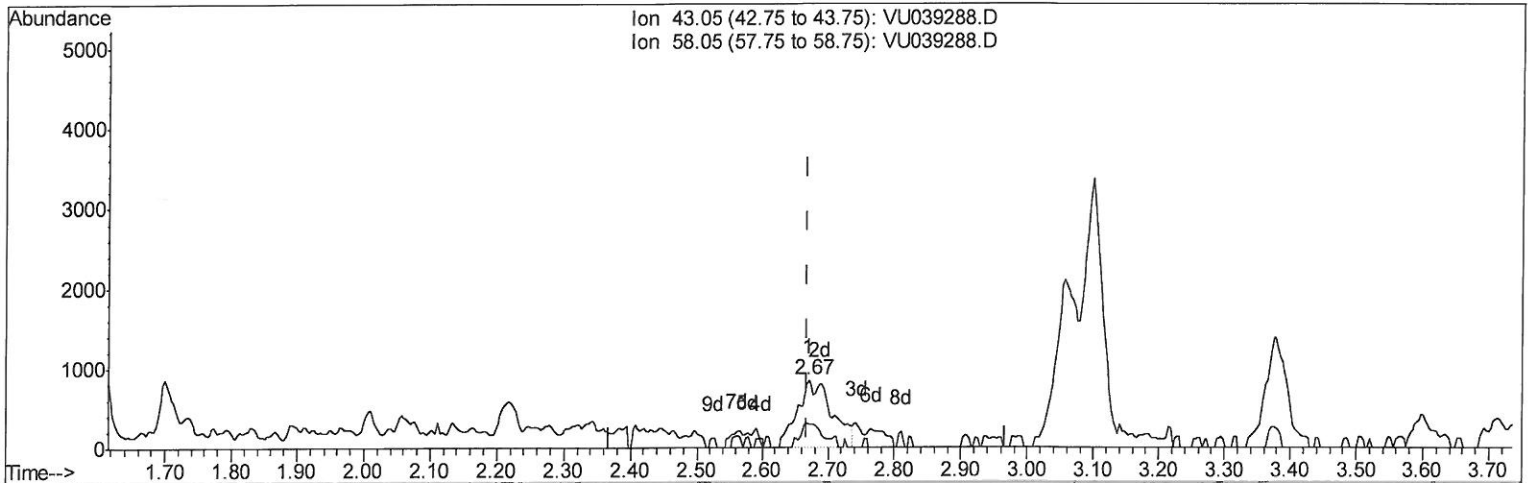

TIC: VU039288.D

(13) Acetone (T)

2.671min (+0.003) 1.81ug/L m

response 3068

Ion	Exp%	Act%
43.05	100	100
58.05	31.80	21.87
0.00	0.00	0.00
0.00	0.00	0.00

2020/07/08 20 54

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070620\
 Data File : VU039288.D
 Acq On : 06 Jul 2020 14:05
 Operator : SY/MD
 Sample : L3193-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4296

Manual Integrations
 APPROVED

MMDadoda
 7/8/2020 2:52:44 PM

Quant Time: Jul 07 01:35:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:17:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	123313	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	116486	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	56343	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	46897	4.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.80%
7) Chloroethane-d5	1.93	69	39940	4.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.20%
11) 1,1-Dichloroethene-d2	2.58	63	66692	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	4.66	46	164435	46.01	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.02%
24) Chloroform-d	5.09	84	85886	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.72	65	53328	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.74	84	177541	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.71	67	57257	4.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.20%
41) Toluene-d8	7.91	98	156855	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
43) trans-1,3-Dichloropropene-	8.19	79	23645	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	8.64	63	134853	46.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.90%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	51361	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	61241	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%

Target Compounds

					Ovalue	
5) Vinyl chloride	1.61	62	38382	4.178	ug/L	# 74
13) Acetone	2.67	43	3068m	1.814	ug/L	76
16) Methylene chloride	3.06	84	933	0.105	ug/L	76
18) trans-1,2-Dichloroethene	3.37	96	6187	0.815	ug/L	90
22) cis-1,2-Dichloroethene	4.69	96	12518	1.447	ug/L	97
30) Cyclohexane	5.41	56	11119	0.830	ug/L	# 93
33) Benzene	5.79	78	8762	0.267	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070620\
Data File : VU039288.D
Acq On : 06 Jul 2020 14:05
Operator : SY/MD
Sample : L3193-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
H4296

Manual Integrations
APPROVED

MMDadoda
7/8/2020 2:52:44 PM

Quant Time: Jul 07 01:35:54 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 07 01:17:04 2020
Response via : Initial Calibration

