

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070620\
 Data File : VU039302.D
 Acq On : 06 Jul 2020 19:28
 Operator : SY/MD
 Sample : VIBLK33
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK33

Quant Time: Jul 07 03:41:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 07 01:17:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	131662	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	122817	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	59755	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	38827	3.83	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.60%
7) Chloroethane-d5	1.92	69	37058	3.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.60%
11) 1,1-Dichloroethene-d2	2.58	63	55335	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	4.66	46	171735	45.00	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.00%
24) Chloroform-d	5.09	84	78324	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.80%
26) 1,2-Dichloroethane-d4	5.72	65	47501	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.20%
32) Benzene-d6	5.75	84	149143	3.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.00%
36) 1,2-Dichloropropane-d6	6.70	67	52012	4.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.80%
41) Toluene-d8	7.91	98	129602	3.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.60%
43) trans-1,3-Dichloropropene-	8.19	79	21867	3.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.40%
46) 2-Hexanone-d5	8.64	63	128625	42.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.04%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	47211	3.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	50943	3.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	75.60%#


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	1217	0.128 ug/L	80




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070620\
Data File : VU039302.D
Acq On : 06 Jul 2020 19:28
Operator : SY/MD
Sample : VIBLK33
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK33

Quant Time: Jul 07 03:41:52 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 07 01:17:04 2020
Response via : Initial Calibration

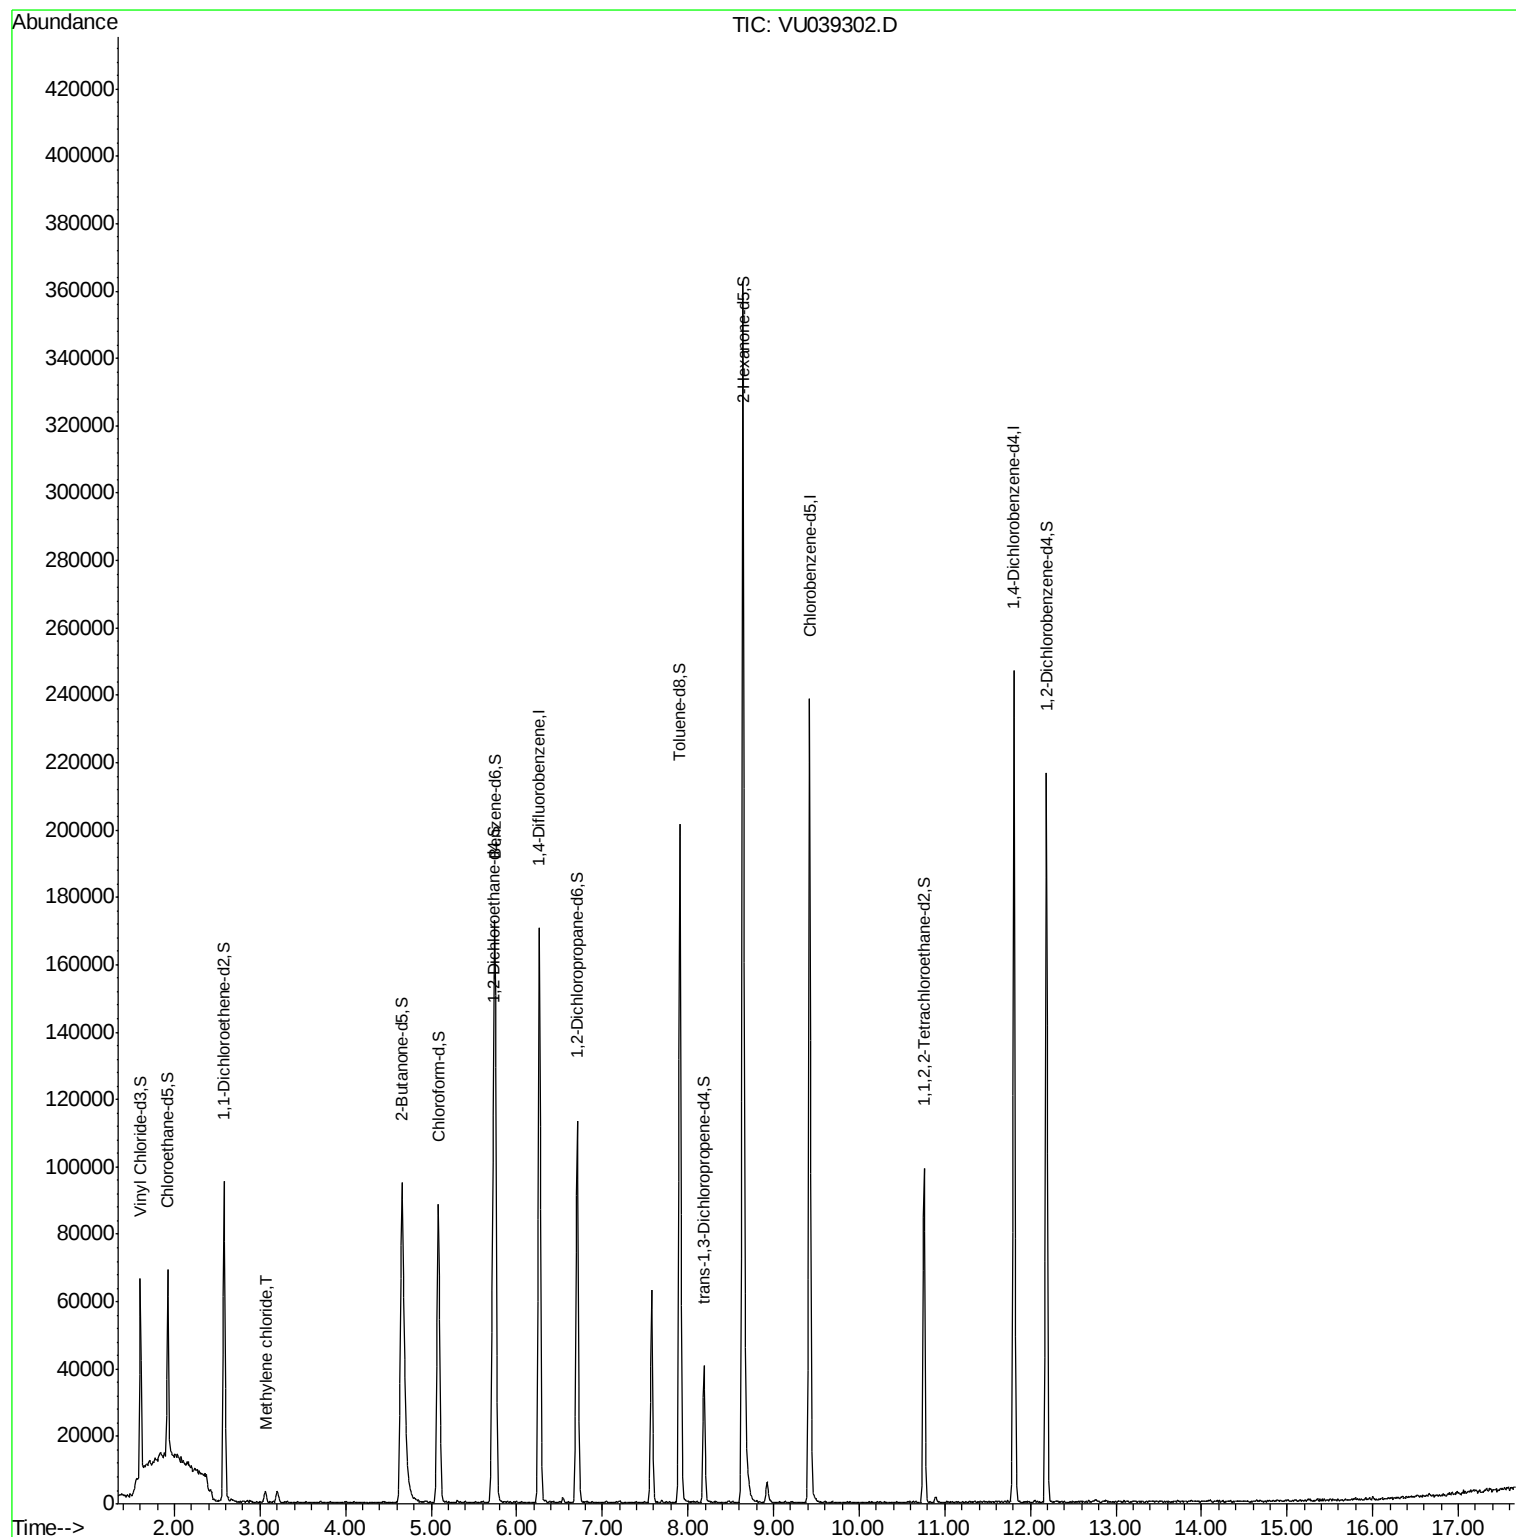

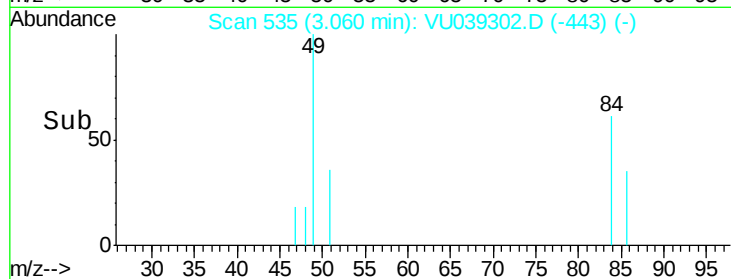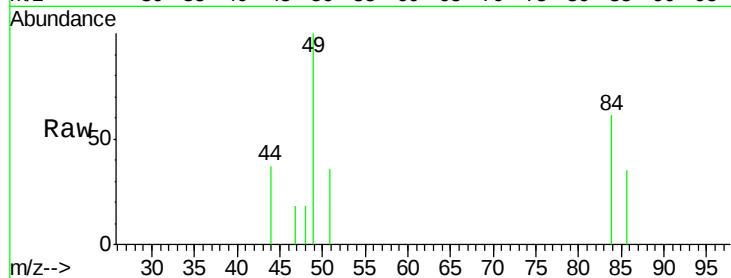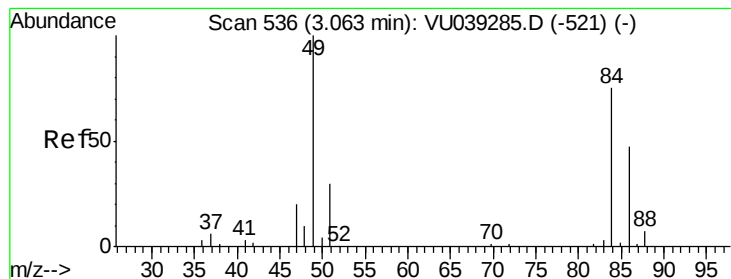

#16
Methylene chloride
Concen: 0.128 ug/L
RT: 3.06 min Scan# 535
Delta R.T. -0.00 min
Lab File: VU039302.D
Acq: 06 Jul 2020 19:28

Instrument :
MSVOA_U
ClientSampleId :
VIBLK33

Tot Ion: 84 Resp: 1217
Ion Ratio Lower Upper
84 100
86 57.3 42.6 79.0
49 165.3 93.0 172.8

