


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070620\
Data File : VU039278.D
Acq On : 06 Jul 2020 08:59
Operator : SY/MD
Sample : BFB25
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070620WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jul 06 09:39:17 2020

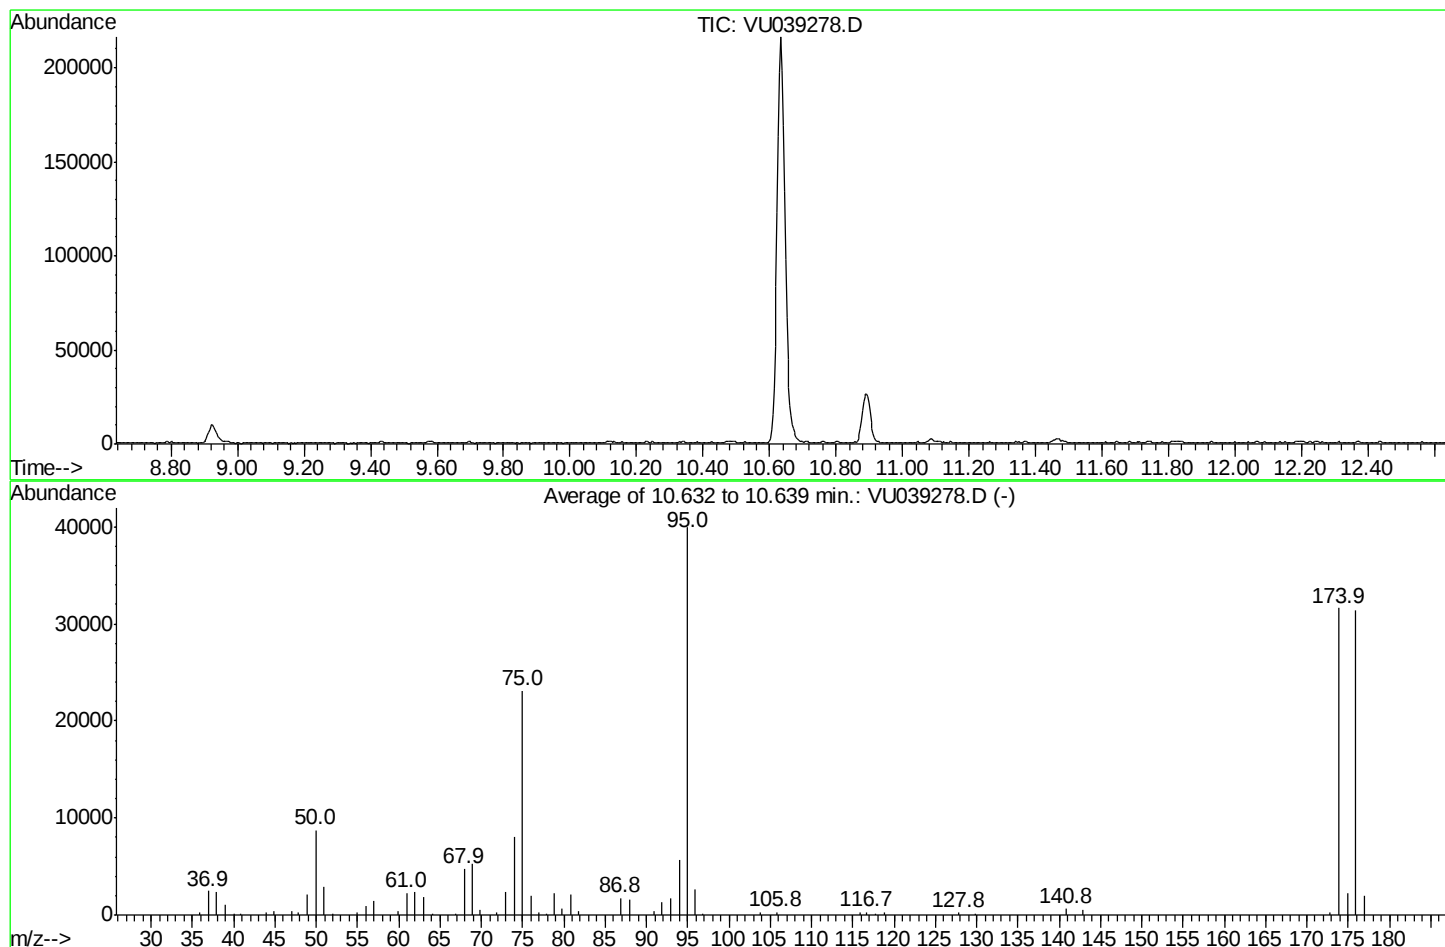

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	8771	PASS
75	95	30	80	57.9	23154	PASS
95	95	100	100	100.0	39957	PASS
96	95	5	9	6.5	2597	PASS
173	174	0.00	2	1.0	321	PASS
174	95	50	120	79.2	31656	PASS
175	174	5	9	7.2	2283	PASS
176	174	95	101	99.1	31381	PASS
177	176	5	9	6.4	2011	PASS

m/z	Abundance
35.90	556.0
36.90	2601.0
37.90	2491.0
38.90	1044.0
40.00	138.0
43.90	571.0
44.90	482.0
47.00	450.0
47.80	265.0
49.00	2421.0
50.00	8786.0
50.90	2805.0
52.00	115.0
54.90	195.0
56.00	978.0
56.90	1589.0
59.90	417.0
60.90	2416.0
61.90	2527.0
63.00	1910.0
64.00	184.0
66.90	166.0
67.90	4999.0
69.00	5401.0
69.90	602.0
71.80	204.0
72.90	2456.0
73.90	8055.0
75.00	24024.0
76.00	2146.0
76.90	249.0
78.00	174.0
78.80	2277.0
79.80	674.0
80.90	2335.0
81.80	429.0
86.80	1879.0
88.00	1653.0
90.80	282.0
91.90	1445.0
93.00	1943.0
94.00	5923.0
95.00	40984.0
95.90	2658.0
96.80	125.0
103.80	236.0
105.80	355.0
115.80	273.0
116.70	340.0
117.80	164.0
118.80	249.0
127.90	202.0
129.80	136.0
140.90	565.0
142.90	585.0
172.90	329.0
173.90	31976.0
174.90	2320.0
175.90	31920.0
176.90	2071.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
35.80	480.0
36.90	2606.0
37.90	2425.0
38.90	1064.0
40.00	204.0
40.90	141.0
43.90	598.0
44.80	458.0
47.00	484.0
47.70	316.0
49.00	2243.0
49.90	9021.0
50.90	2969.0
52.00	123.0
54.90	246.0
56.00	923.0
56.90	1604.0
59.90	461.0
60.90	2326.0
61.90	2518.0
62.90	1881.0
64.00	189.0
66.90	112.0
67.90	4900.0
69.00	5375.0
69.90	560.0
71.80	287.0
72.90	2474.0
74.00	8181.0
75.00	23568.0
76.00	2027.0
77.00	243.0
77.90	140.0
78.80	2351.0
79.80	633.0
80.80	2136.0
81.80	432.0
86.80	1833.0
87.90	1643.0
90.80	359.0
91.90	1315.0
92.90	1758.0
93.90	5902.0
95.00	41328.0
95.90	2694.0
96.80	118.0
103.80	252.0
105.80	336.0
115.90	266.0
116.70	346.0
117.80	171.0
118.80	238.0
127.80	239.0
129.80	143.0
140.90	695.0
142.90	573.0
172.80	333.0
173.90	32520.0
174.90	2325.0
175.90	32240.0
176.90	2070.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
35.80	486.0
36.90	2294.0
37.90	2119.0
38.90	934.0
40.00	188.0
40.90	166.0
44.00	651.0
44.80	440.0
47.00	458.0
47.70	313.0
48.90	1867.0
49.90	8508.0
50.90	2881.0
52.00	156.0
54.90	237.0
56.00	819.0
56.90	1438.0
59.90	441.0
61.00	2081.0
61.90	2277.0
62.90	1691.0
64.10	176.0
67.90	4455.0
68.90	4946.0
69.90	474.0
71.80	296.0
72.90	2248.0
73.90	7753.0
75.00	21872.0
76.00	1709.0
76.90	244.0
77.80	131.0
78.90	2229.0
79.80	568.0
80.80	1966.0
81.80	406.0
86.90	1581.0
87.90	1469.0
90.90	385.0
91.90	1167.0
92.90	1514.0
93.90	5191.0
95.00	37560.0
95.90	2440.0
103.90	243.0
105.80	297.0
115.90	250.0
116.70	308.0
117.80	130.0
118.80	209.0
127.80	226.0
129.90	145.0
140.80	657.0
142.80	483.0
172.70	303.0
173.90	30472.0
174.90	2206.0
175.90	29984.0
176.90	1894.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Scan 2877 (10.590 min): VU039278.D
BFB25

m/z	Abundance
35.80	227.0
39.70	155.0
43.90	356.0
57.00	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25