

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070622\
 Data File : VU049637.D
 Acq On : 06 Jul 2022 16:17
 Operator : SY/MD
 Sample : VU0706WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0706WBL01

Quant Time: Jul 07 07:20:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 07 07:00:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.115	96	37179	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	12418	0.912	ug/l	0.00
Spiked Amount 1.000			Recovery	=	91.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	12370	0.987	ug/l	0.00
Spiked Amount 1.000			Recovery	=	99.000%	
Target Compounds						
15) Methylene Chloride	3.041	84	9522	0.902	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070622\
Data File : VU049637.D
Acq On : 06 Jul 2022 16:17
Operator : SY/MD
Sample : VU0706WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0706WBL01


Quant Time: Jul 07 07:20:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 07 07:00:33 2022
Response via : Initial Calibration

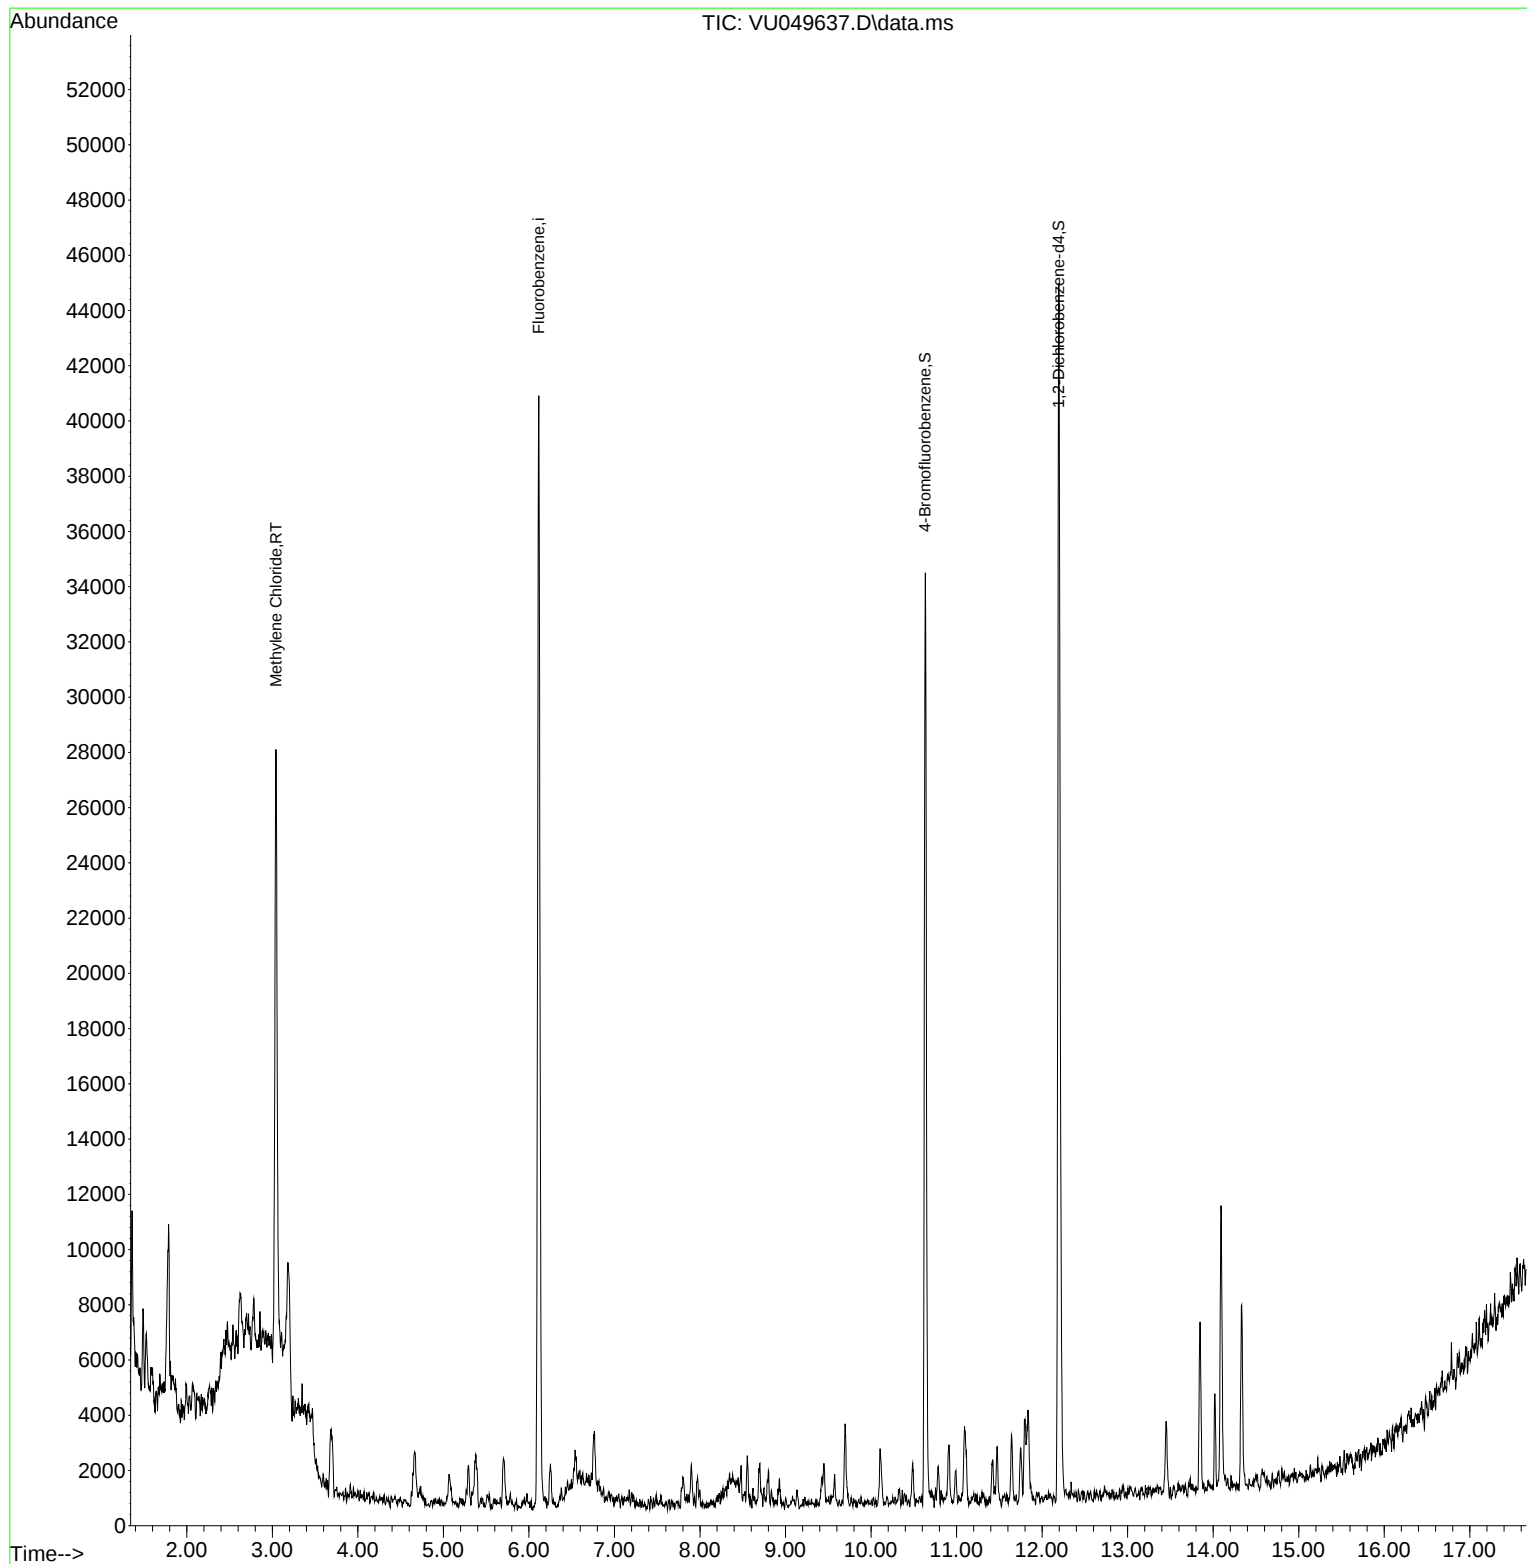

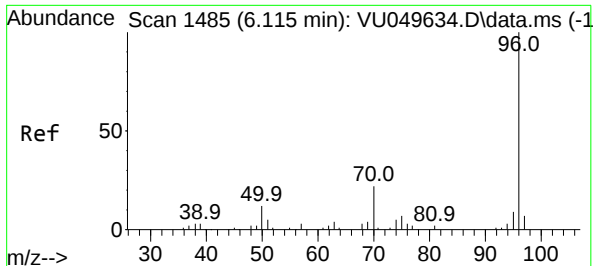




#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1485
Delta R.T. -0.000 min
Lab File: VU049637.D
Acq: 06 Jul 2022 16:17

Instrument :
MSVOA_U
ClientSampleId :
VU0706WBL01

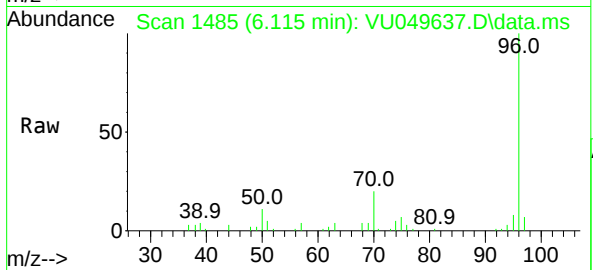


Tgt Ion: 96 Resp: 37179

Ion	Ratio	Lower	Upper
96	100		
70	21.3	16.7	25.1
95	8.0	7.4	11.0
97	6.3	0.0	0.0

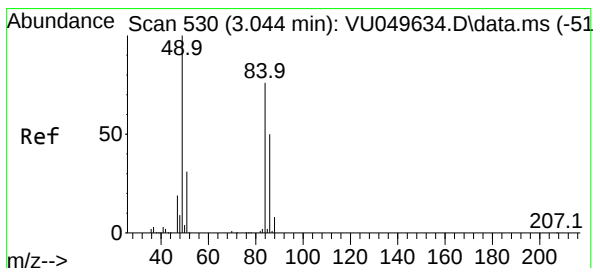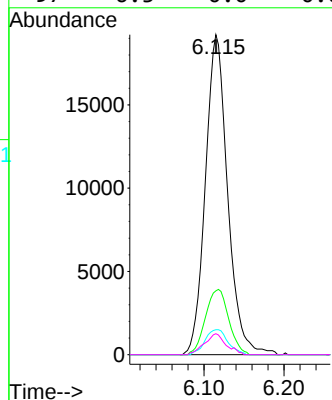
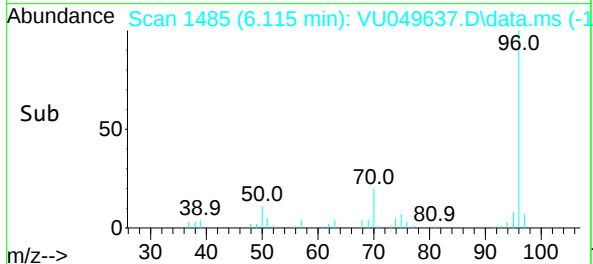



#15
Methylene Chloride
Concen: 0.902 ug/l
RT: 3.041 min Scan# 529
Delta R.T. -0.003 min
Lab File: VU049637.D
Acq: 06 Jul 2022 16:17

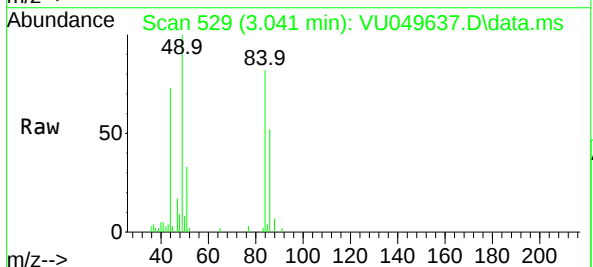

Tgt Ion: 84 Resp: 9522

Ion	Ratio	Lower	Upper
84	100		
49	122.4	104.6	157.0
51	40.4	0.0	81.4
86	64.1	52.6	78.8



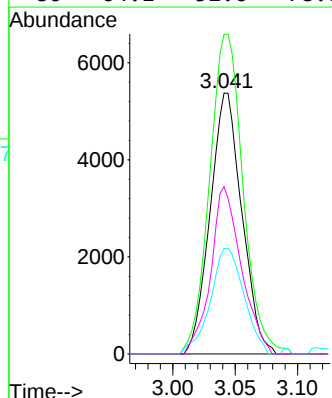
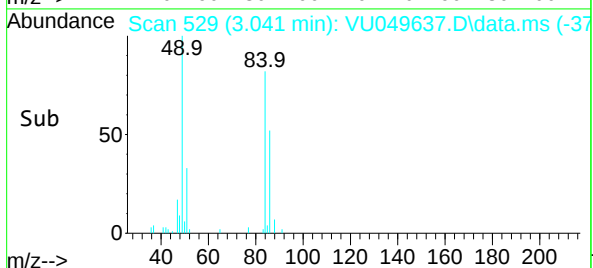


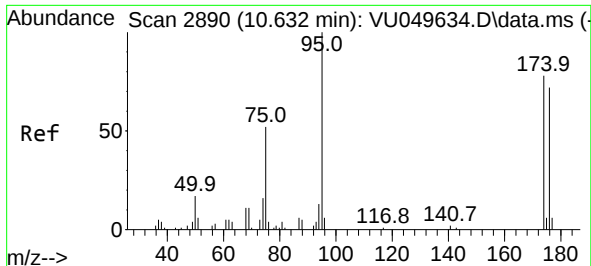

#57
4-Bromofluorobenzene
Concen: 0.912 ug/l
RT: 10.632 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU049637.D
Acq: 06 Jul 2022 16:17

Instrument :
MSVOA_U
ClientSampleId :
VU0706WBL01

Tgt Ion: 95 Resp: 12418
Ion Ratio Lower Upper
95 100
174 76.5 62.4 93.6
176 74.1 56.2 84.2

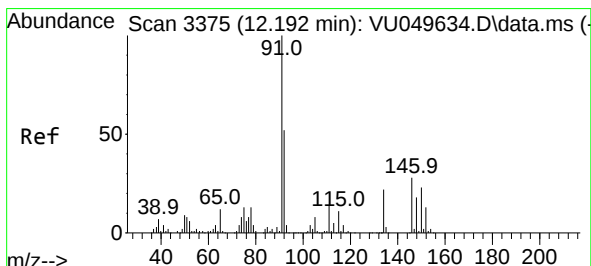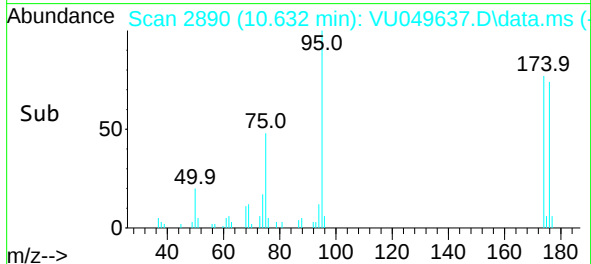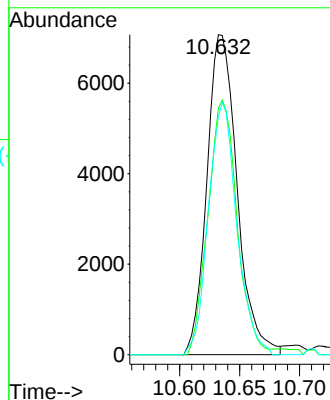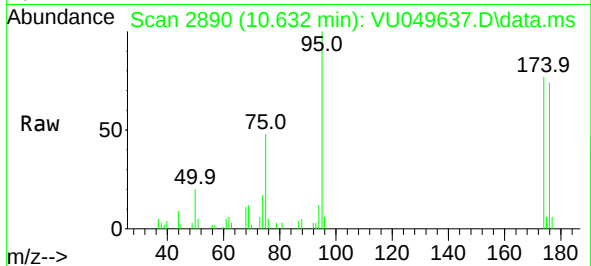

#68
1,2-Dichlorobenzene-d4
Concen: 0.987 ug/l
RT: 12.195 min Scan# 3376
Delta R.T. 0.003 min
Lab File: VU049637.D
Acq: 06 Jul 2022 16:17

Tgt Ion: 152 Resp: 12370
Ion Ratio Lower Upper
152 100
115 68.9 0.0 254.6
150 157.8 0.0 623.6

