


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070622\
Data File : VU049629.D
Acq On : 06 Jul 2022 08:48
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jul 07 07:00:33 2022

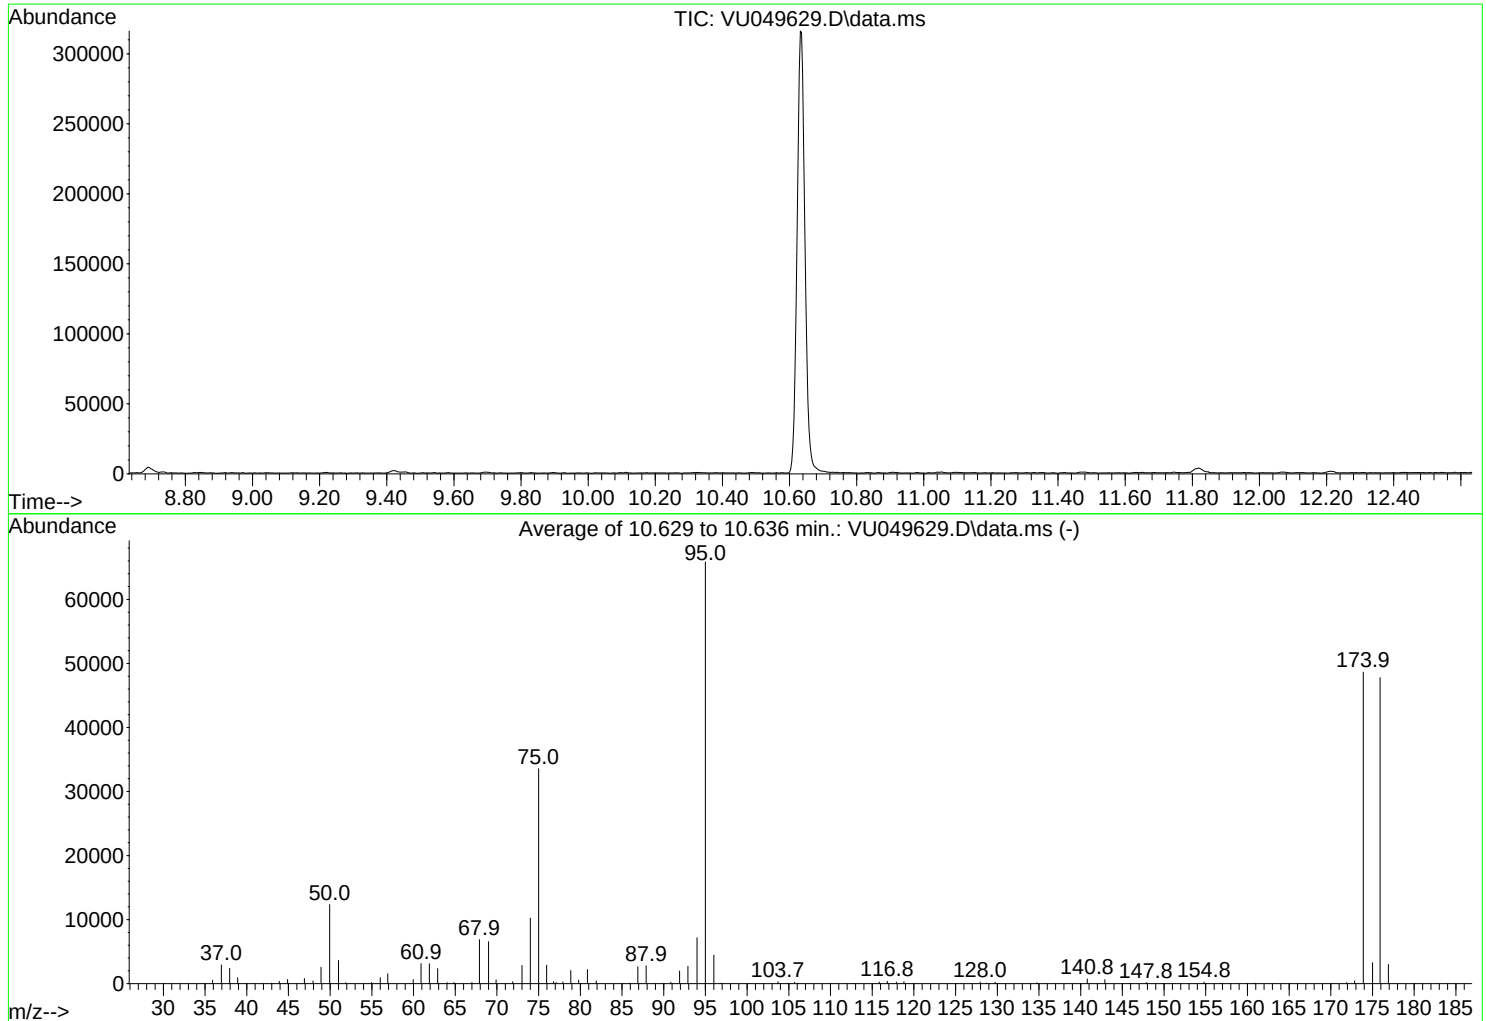

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	12337	PASS
75	95	30	60	50.9	33552	PASS
95	95	100	100	100.0	65864	PASS
96	95	5	9	6.8	4454	PASS
173	174	0.00	2	0.9	428	PASS
174	95	50	100	73.9	48648	PASS
175	174	5	9	6.7	3264	PASS
176	174	95	101	98.2	47795	PASS
177	176	5	9	6.3	2996	PASS