

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070721\
 Data File : VU044318.D
 Acq On : 07 Jul 2021 16:35
 Operator : SY/MD
 Sample : VU0707WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0707WBL01

Quant Time: Jul 08 01:44:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 08 01:42:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.124	96	27064	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	11510	0.960	ug/l	0.00
Spiked Amount 1.000			Recovery	=	96.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	11258	0.942	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070721\
Data File : VU044318.D
Acq On : 07 Jul 2021 16:35
Operator : SY/MD
Sample : VU0707WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0707WBL01

Quant Time: Jul 08 01:44:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 08 01:42:26 2021
Response via : Initial Calibration

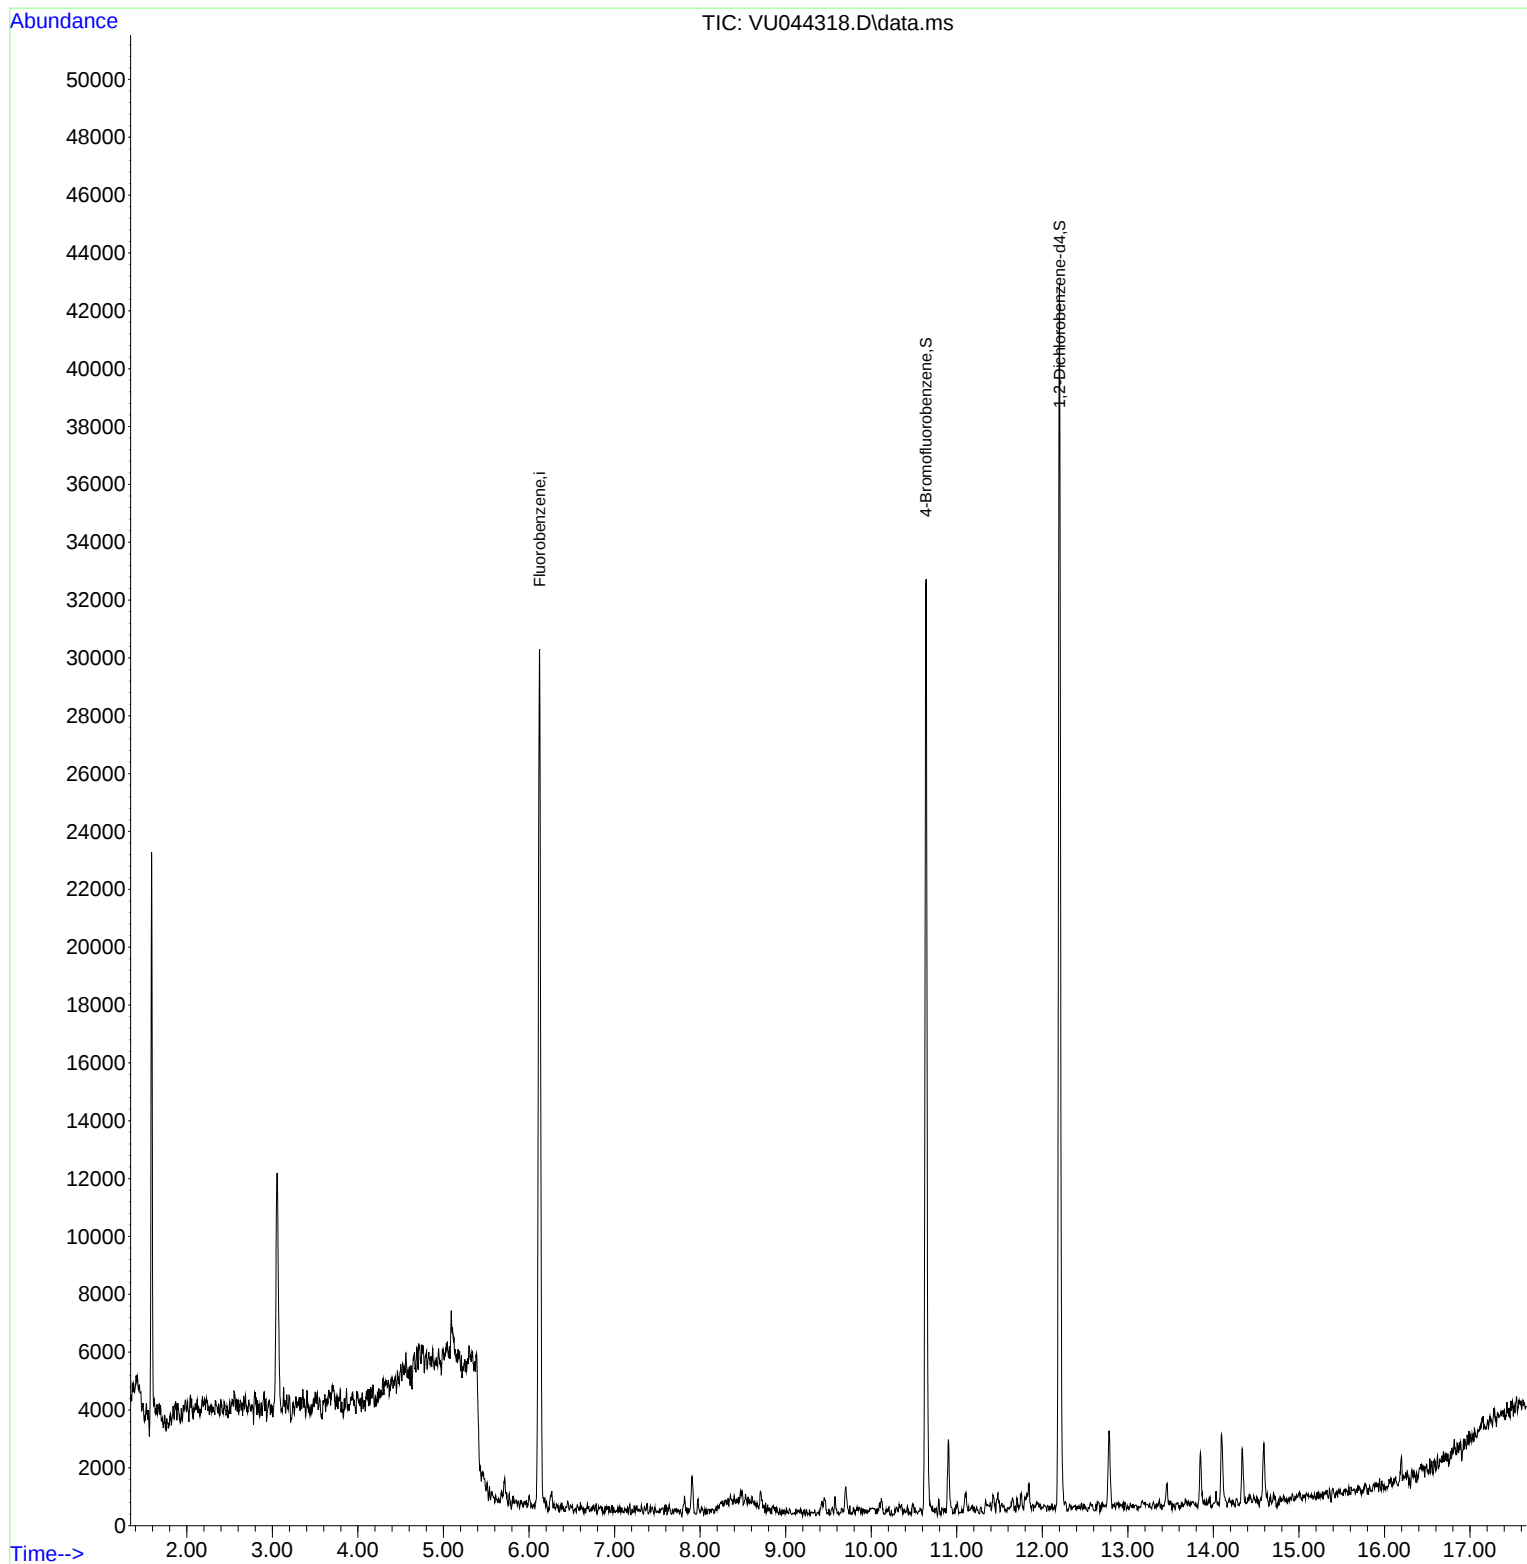




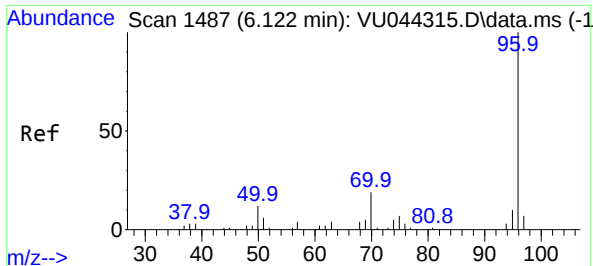


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.124 min Scan# 1488
Delta R.T. 0.002 min
Lab File: VU044318.D
Acq: 07 Jul 2021 16:35

Instrument :
MSVOA_U
ClientSampleId :
VU0707WBL01

Tgt Ion: 96 Resp: 27064




Ion	Ratio	Lower	Upper
96	100		
70	19.9	16.2	24.2
95	8.4	7.3	10.9
97	6.4	0.0	0.0

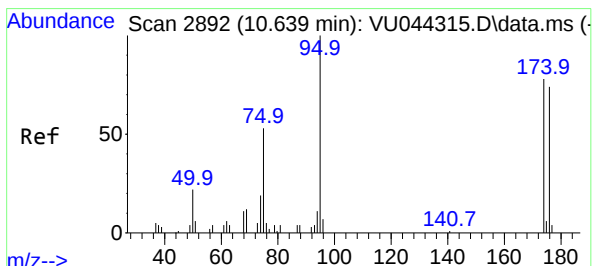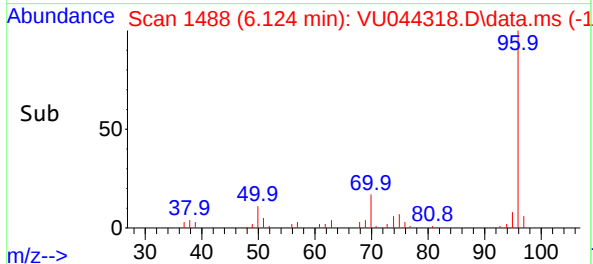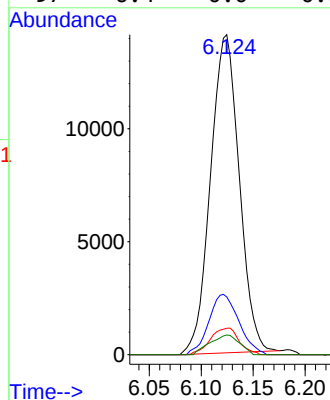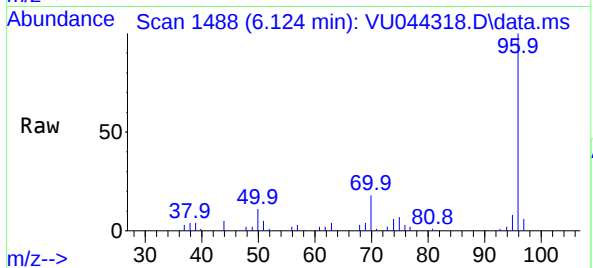


#57
4-Bromofluorobenzene
Concen: 0.960 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU044318.D
Acq: 07 Jul 2021 16:35

Tgt Ion: 95 Resp: 11510

Ion	Ratio	Lower	Upper
95	100		
174	78.1	62.2	93.2
176	76.0	60.3	90.5

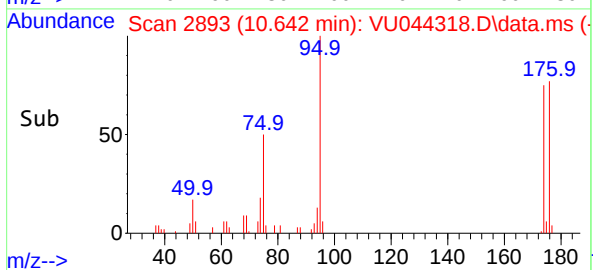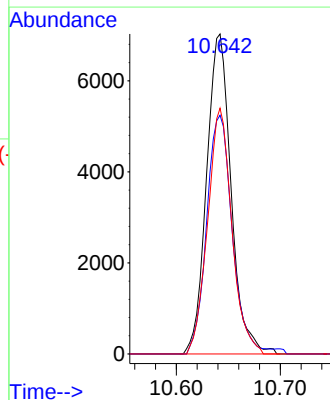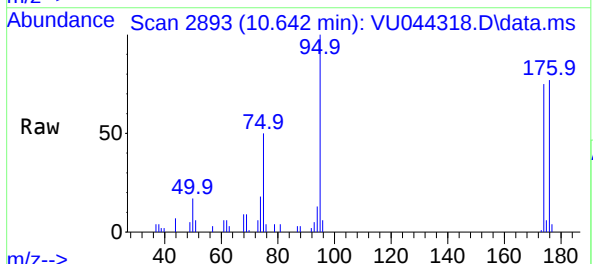

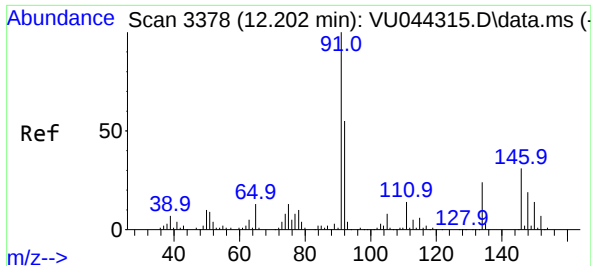

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.942 ug/l
 RT: 12.201 min Scan# 3378
 Delta R.T. -0.000 min
 Lab File: VU044318.D
 Acq: 07 Jul 2021 16:35

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0707WBL01

Tgt Ion:152	Resp:	11258
Ion Ratio	Lower	Upper
152	100	
115	69.3	0.0 257.0
150	160.1	0.0 630.2

