


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070721\
Data File : VU044310.D
Acq On : 07 Jul 2021 09:52
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jul 08 15:34:52 2021

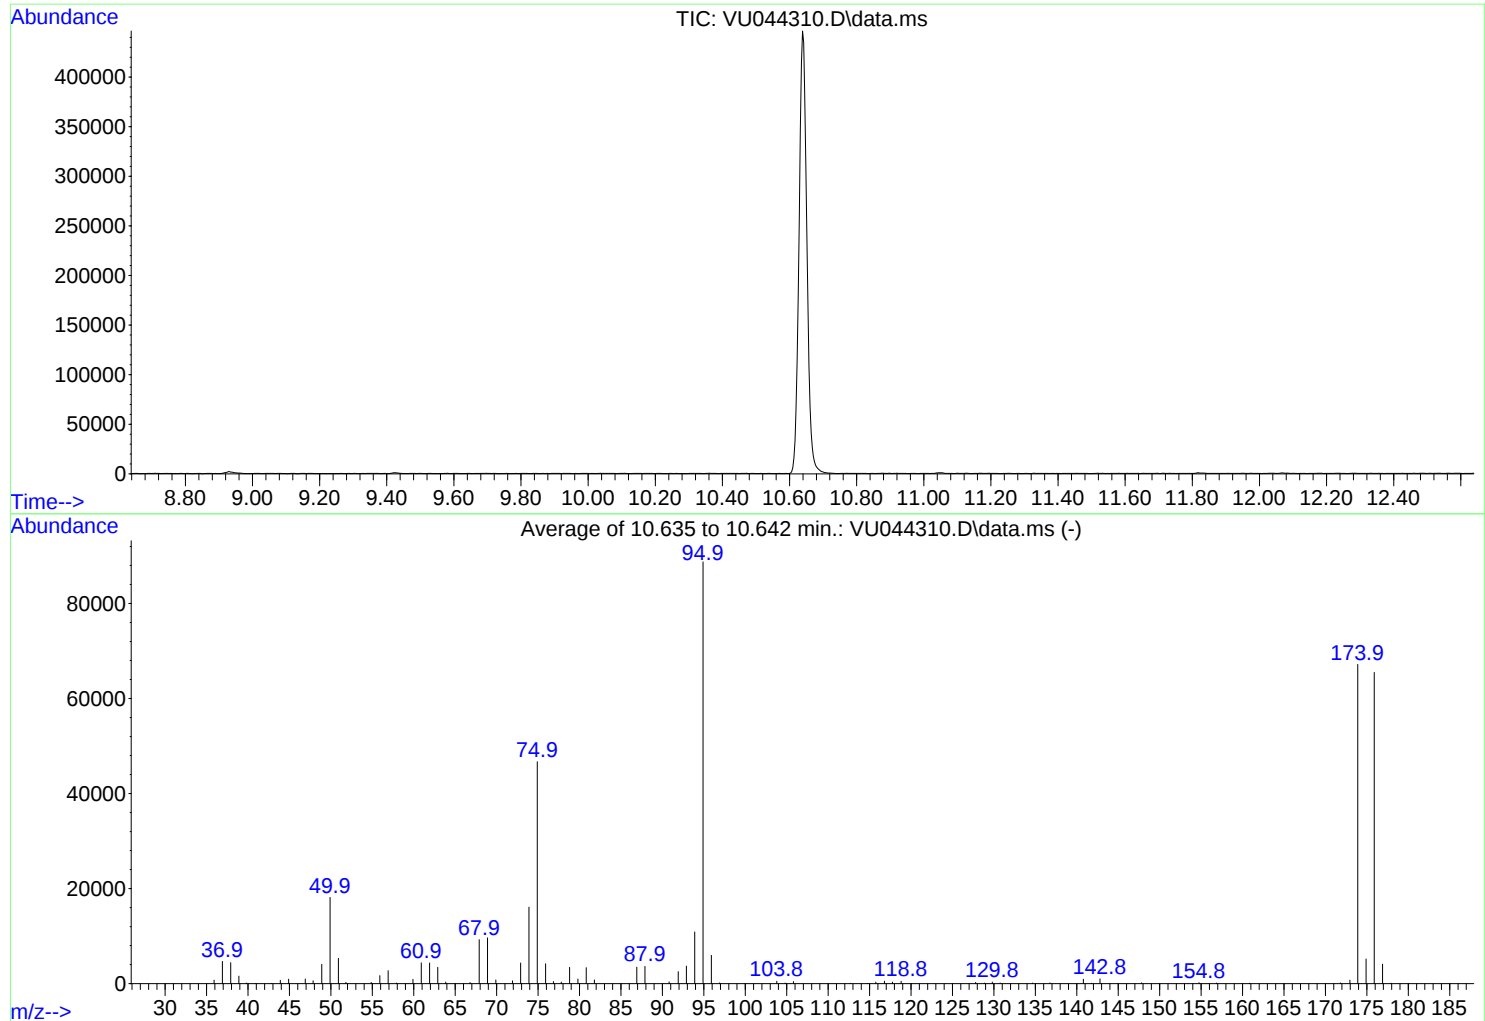

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	18141	PASS
75	95	30	60	52.6	46699	PASS
95	95	100	100	100.0	88760	PASS
96	95	5	9	6.7	5944	PASS
173	174	0.00	2	1.1	734	PASS
174	95	50	100	75.7	67171	PASS
175	174	5	9	7.7	5195	PASS
176	174	95	101	97.5	65499	PASS
177	176	5	9	6.3	4124	PASS