

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070722\
 Data File : VU049646.D
 Acq On : 07 Jul 2022 11:29
 Operator : SY/MD
 Sample : VU0707WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0707WBL01

Quant Time: Jul 08 09:11:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 07 07:00:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	41826	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	13066	0.853	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	12625	0.895	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070722\
Data File : VU049646.D
Acq On : 07 Jul 2022 11:29
Operator : SY/MD
Sample : VU0707WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0707WBL01

Quant Time: Jul 08 09:11:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 07 07:00:33 2022
Response via : Initial Calibration

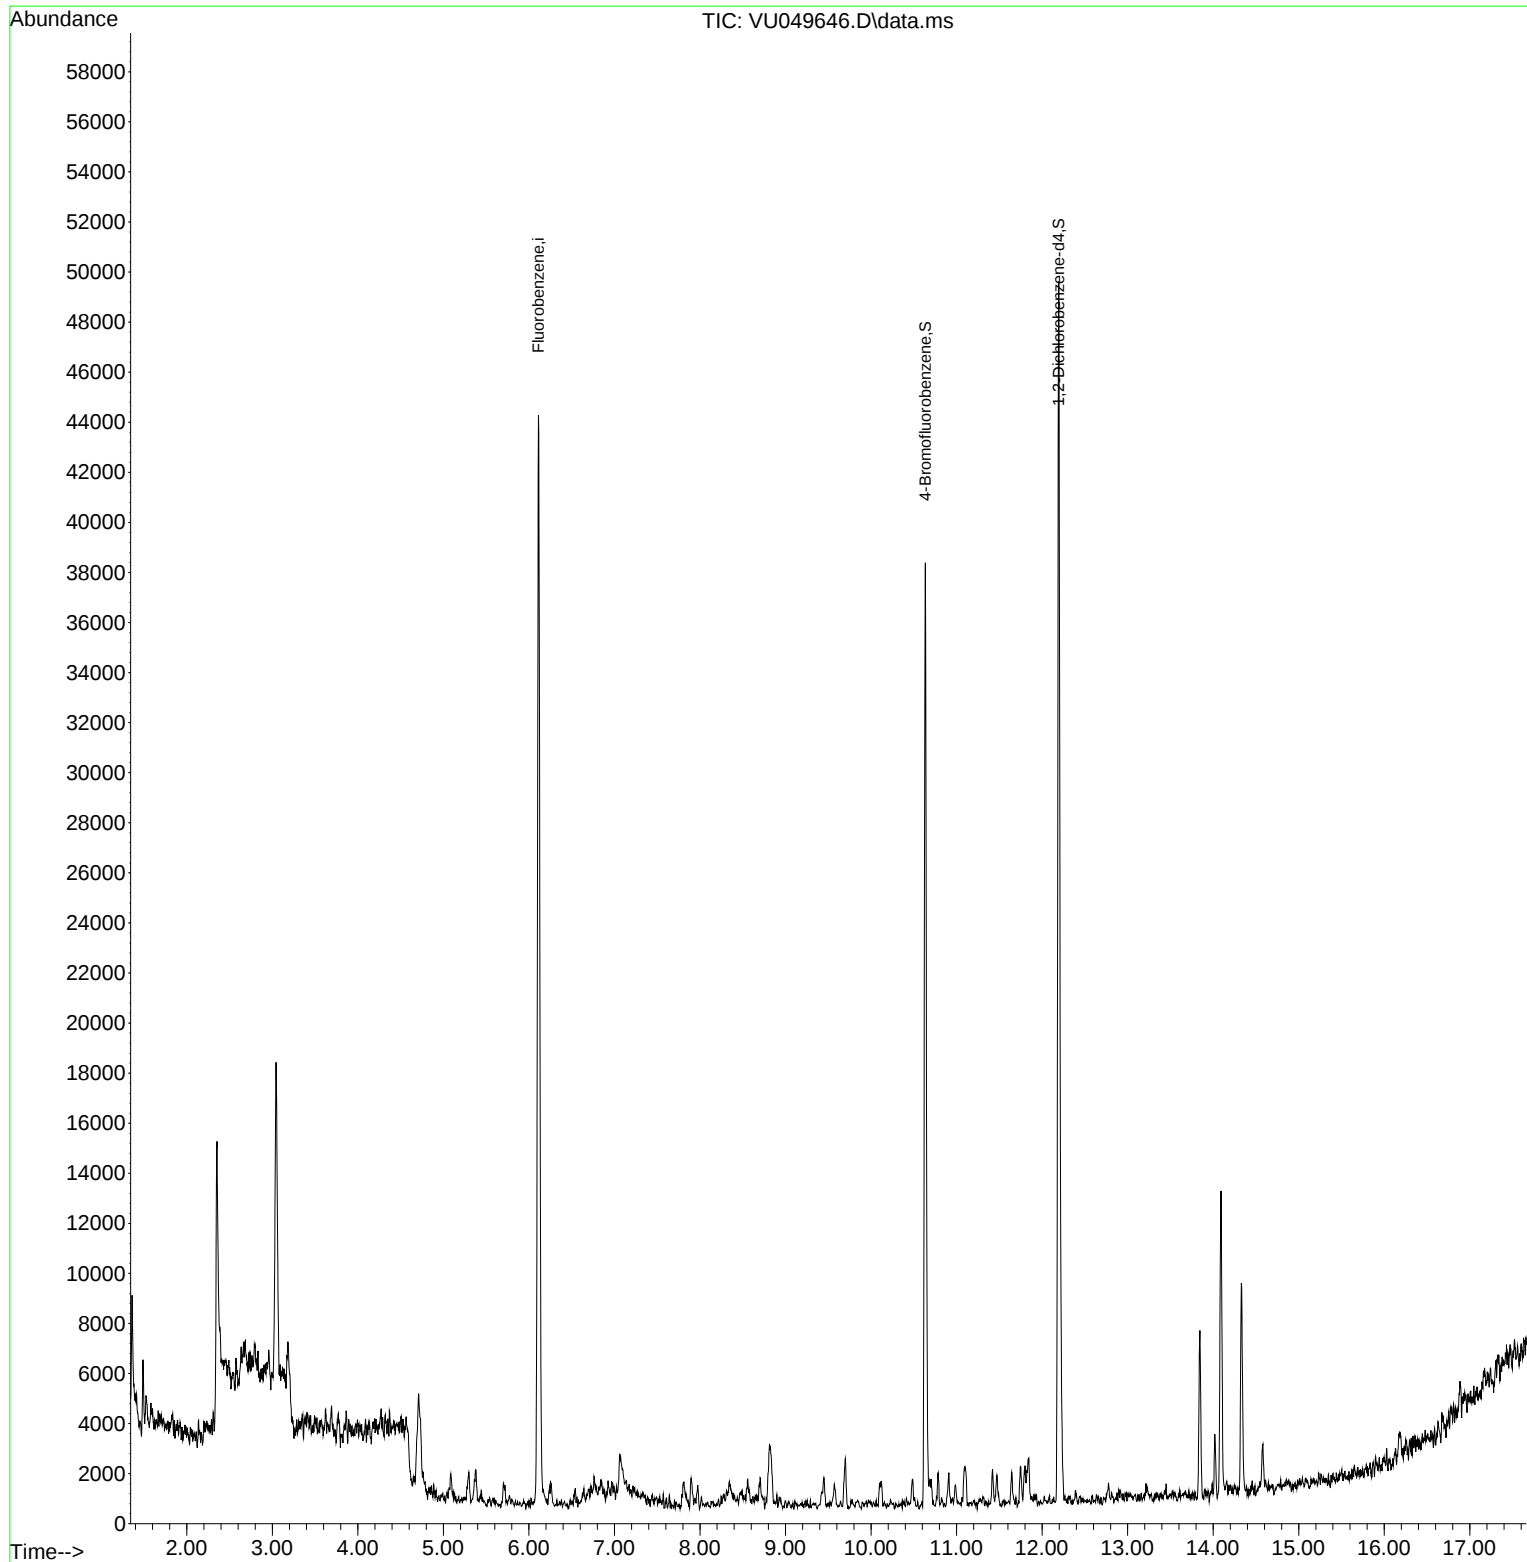




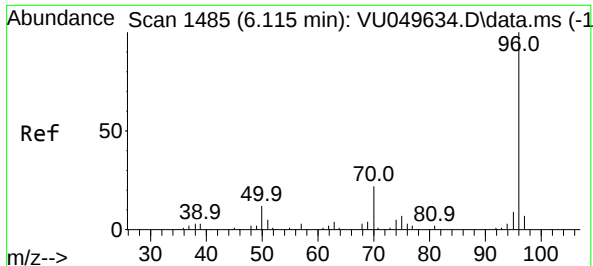


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1485
Delta R.T. -0.003 min
Lab File: VU049646.D
Acq: 07 Jul 2022 11:29

Instrument :
MSVOA_U
ClientSampleId :
VU0707WBL01

Tgt Ion: 96 Resp: 41826




Ion	Ratio	Lower	Upper
96	100		
70	19.9	16.7	25.1
95	8.0	7.4	11.0
97	6.6	0.0	0.0

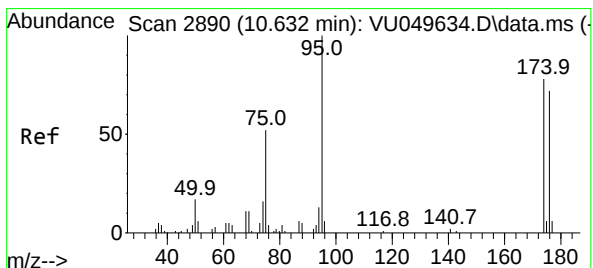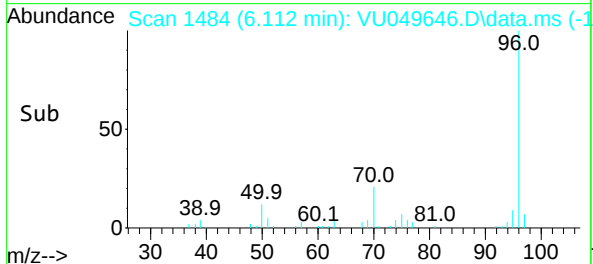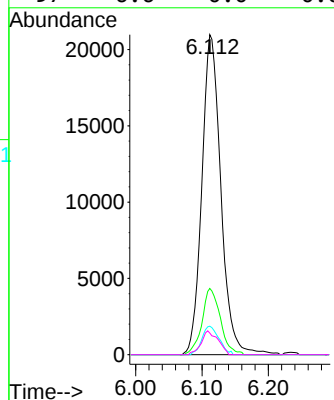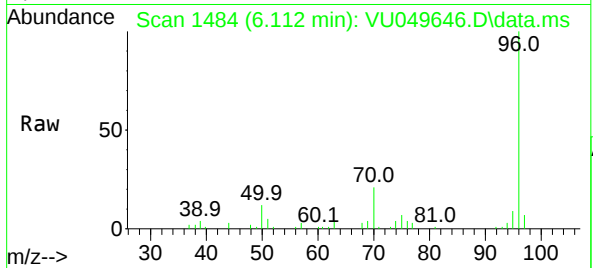


#57
4-Bromofluorobenzene
Concen: 0.853 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU049646.D
Acq: 07 Jul 2022 11:29

Tgt Ion: 95 Resp: 13066


Ion	Ratio	Lower	Upper
95	100		
174	79.7	62.4	93.6
176	76.7	56.2	84.2

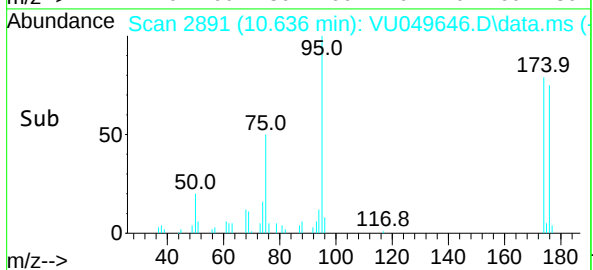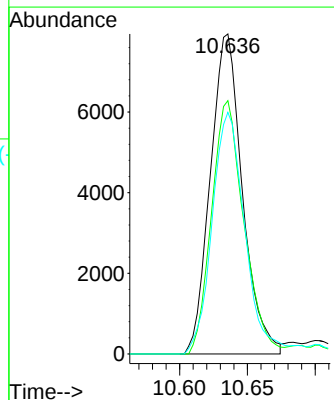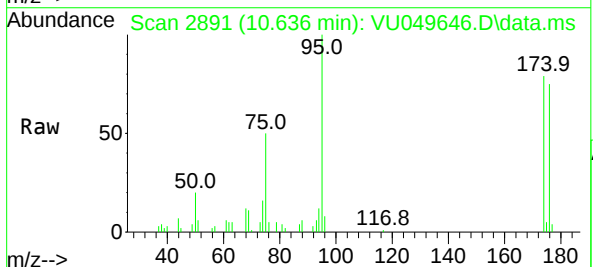

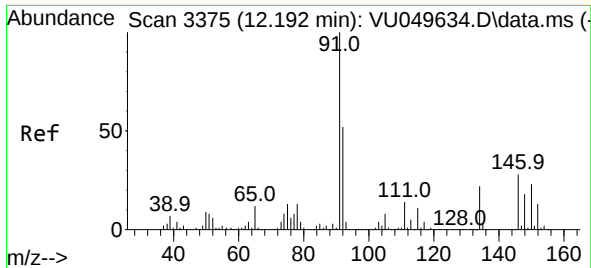

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.895 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU049646.D
 Acq: 07 Jul 2022 11:29

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0707WBL01

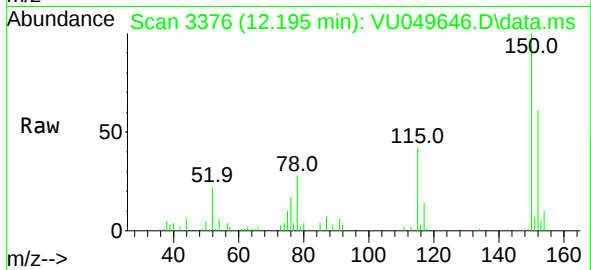

Tgt Ion	Ratio	Lower	Upper
152	100		
115	71.7	0.0	254.6
150	166.2	0.0	623.6

