


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070723\
Data File : VU054770.D
Acq On : 07 Jul 2023 08:40
Operator : MD/SY
Sample : BFB031
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB031

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR070723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jul 08 07:50:39 2023

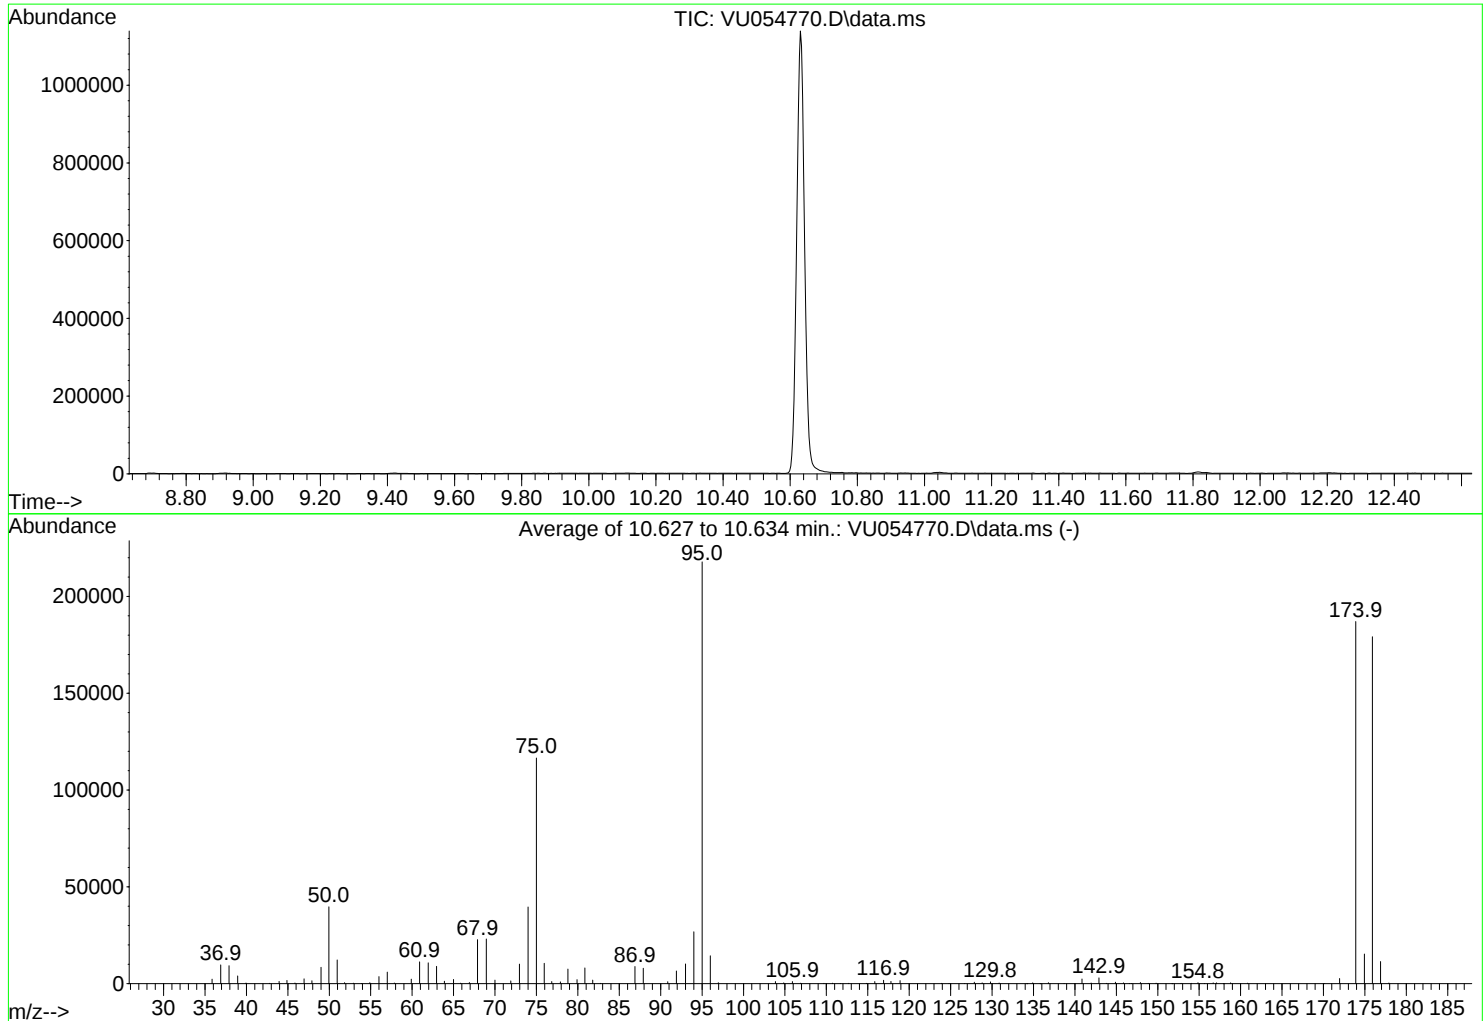

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	39635	PASS
75	95	30	80	53.5	116496	PASS
95	95	100	100	100.0	217856	PASS
96	95	5	9	6.6	14370	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.8	187029	PASS
175	174	5	9	8.2	15269	PASS
176	174	95	101	95.8	179200	PASS
177	176	5	9	6.4	11401	PASS

m/z	Abundance
35.80	546.0
37.90	174.0
39.70	107.0
43.80	448.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	3047.0
36.90	9906.0
38.00	9580.0
39.00	3761.0
40.00	383.0
42.80	190.0
44.00	1608.0
44.90	1731.0
46.00	340.0
46.90	2544.0
47.90	1301.0
49.00	8295.0
50.00	39760.0
51.00	12048.0
51.90	558.0
52.90	243.0
54.90	482.0
56.00	3362.0
57.00	6094.0
57.90	318.0
59.90	2392.0
60.90	11488.0
62.00	10571.0
62.90	8789.0
63.90	1308.0
65.00	2007.0
65.90	282.0
66.90	625.0
67.90	22672.0
69.00	22840.0
70.00	1961.0
71.90	1433.0
72.90	9624.0
74.00	38296.0
75.00	114104.0
76.00	10435.0
76.90	1165.0
77.90	846.0
78.80	7231.0
79.90	2017.0
80.90	7920.0
81.80	1747.0
82.70	169.0
86.90	8964.0
87.90	7644.0
90.90	988.0
91.90	6307.0
93.00	9760.0
94.00	26296.0
95.00	211648.0
96.00	14135.0
97.00	478.0
103.80	902.0
104.90	370.0
105.90	1063.0
106.90	242.0
109.70	169.0
110.00	190.0
110.90	260.0
112.60	168.0
114.80	207.0
115.90	984.0
116.90	1725.0
117.80	1170.0
118.90	1602.0
123.90	248.0
127.80	830.0
128.80	399.0
129.80	904.0
130.90	330.0
134.90	424.0
135.80	103.0
136.80	488.0
138.70	100.0
140.90	2185.0
141.90	311.0
142.90	2981.0
143.80	166.0
144.90	702.0
145.90	317.0
146.60	159.0
147.90	575.0
148.90	150.0
149.80	288.0
152.80	223.0
154.10	225.0
154.90	535.0
155.60	136.0
156.70	424.0
157.10	314.0
157.90	114.0
158.80	341.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

160.90	206.0
171.90	2613.0
173.90	179520.0
175.00	14675.0
175.90	170752.0
176.90	11401.0
177.90	336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	2910.0
36.90	9804.0
37.90	9803.0
38.90	4086.0
40.00	356.0
42.80	189.0
44.00	1681.0
44.90	1719.0
45.80	355.0
46.90	2602.0
47.90	1576.0
49.00	8655.0
50.00	40584.0
50.90	12446.0
51.90	496.0
52.90	244.0
53.90	108.0
54.90	540.0
56.00	3685.0
57.00	6125.0
57.80	399.0
59.90	2405.0
60.90	11497.0
62.00	11017.0
63.00	9165.0
63.90	1331.0
65.00	2247.0
65.80	339.0
66.90	563.0
67.90	23488.0
69.00	23728.0
70.00	1913.0
71.90	1427.0
72.90	10380.0
74.00	41048.0
75.00	120408.0
76.00	10921.0
76.90	1031.0
77.90	948.0
78.80	7624.0
79.90	2184.0
80.90	8390.0
81.80	1833.0
82.80	206.0
86.90	9075.0
87.90	8213.0
90.90	1010.0
91.90	6656.0
93.00	10603.0
94.00	27416.0
95.00	225344.0
96.00	14727.0
96.90	593.0
103.80	1097.0
104.80	428.0
105.90	1182.0
106.90	273.0
109.70	206.0
110.70	253.0
111.70	156.0
112.70	148.0
114.90	161.0
115.90	1099.0
116.90	1751.0
117.80	1230.0
118.90	1579.0
123.90	184.0
124.80	108.0
127.80	818.0
128.80	392.0
129.80	891.0
130.90	330.0
134.90	444.0
136.80	568.0
138.70	102.0
140.90	2456.0
141.90	339.0
142.90	3102.0
143.80	188.0
144.90	768.0
145.80	440.0
146.80	119.0
147.90	592.0
148.80	176.0
149.80	269.0
152.80	203.0
154.10	186.0
154.80	552.0
155.70	121.0
156.70	441.0
157.10	448.0
158.80	444.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

160.80	269.0
170.10	100.0
171.90	2699.0
173.90	192896.0
174.90	15779.0
175.90	185152.0
176.90	11722.0
177.90	321.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	2536.0
36.90	9228.0
37.90	9005.0
39.00	4040.0
39.90	281.0
42.80	185.0
44.00	1619.0
44.90	1650.0
45.80	310.0
47.00	2399.0
47.90	1568.0
49.00	8272.0
49.90	38560.0
51.00	12313.0
51.80	431.0
52.90	225.0
53.90	141.0
54.90	579.0
56.00	3791.0
57.00	5747.0
57.80	403.0
59.90	2190.0
60.90	10676.0
61.90	10641.0
63.00	8829.0
63.90	1150.0
65.00	2269.0
65.80	257.0
66.90	490.0
67.90	22000.0
68.90	22648.0
70.00	1688.0
71.90	1280.0
73.00	10278.0
74.00	39352.0
75.00	114976.0
75.90	10079.0
76.80	977.0
77.90	861.0
78.80	7690.0
79.90	2115.0
80.80	8029.0
81.80	1778.0
82.80	211.0
86.90	8548.0
87.90	8002.0
90.80	931.0
91.90	6690.0
93.00	10245.0
94.00	26552.0
95.00	216576.0
96.00	14247.0
96.90	497.0
103.90	1189.0
104.90	403.0
105.90	1063.0
106.90	204.0
109.70	176.0
110.60	222.0
111.70	181.0
112.80	153.0
114.80	168.0
115.80	1106.0
116.90	1690.0
117.80	1203.0
118.90	1468.0
123.90	133.0
124.80	133.0
126.70	146.0
127.90	707.0
128.80	345.0
129.80	894.0
130.80	360.0
134.20	117.0
134.90	479.0
136.80	542.0
140.00	253.0
140.80	2451.0
142.00	396.0
142.90	2844.0
143.80	234.0
144.90	757.0
145.80	531.0
146.90	126.0
147.90	581.0
148.80	201.0
149.80	227.0
151.70	112.0
152.80	144.0
153.90	157.0
154.80	495.0
156.70	368.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

157.10	440.0
158.80	403.0
160.90	288.0
170.10	147.0
172.00	2698.0
173.90	188672.0
174.90	15353.0
175.90	181696.0
176.90	11080.0
177.90	278.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031