

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070820\
 Data File : VU039374.D
 Acq On : 09 Jul 2020 02:44
 Operator : SY/MD
 Sample : L3243-18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A85

Quant Time: Jul 09 07:35:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 09 05:48:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	102371	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	95234	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	44993	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	25901	4.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.40%
7) Chloroethane-d5	1.93	69	30762	5.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.40%
11) 1,1-Dichloroethene-d2	2.58	63	41973	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.00%
20) 2-Butanone-d5	4.65	46	146827	54.08	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.16%
24) Chloroform-d	5.08	84	62488	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.72	65	41571	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.75	84	124320	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.40%
36) 1,2-Dichloropropane-d6	6.71	67	42767	5.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.20%
41) Toluene-d8	7.91	98	107630	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.40%
43) trans-1,3-Dichloropropene-	8.19	79	16586	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.64	63	108213	51.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.58%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	39396	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	44032	5.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.60%


Target Compounds				Ovalue
13) Acetone	2.66	43	3776	2.577 ug/L 92




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU070820\
Data File : VU039374.D
Acq On : 09 Jul 2020 02:44
Operator : SY/MD
Sample : L3243-18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A85

Quant Time: Jul 09 07:35:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 09 05:48:41 2020
Response via : Initial Calibration

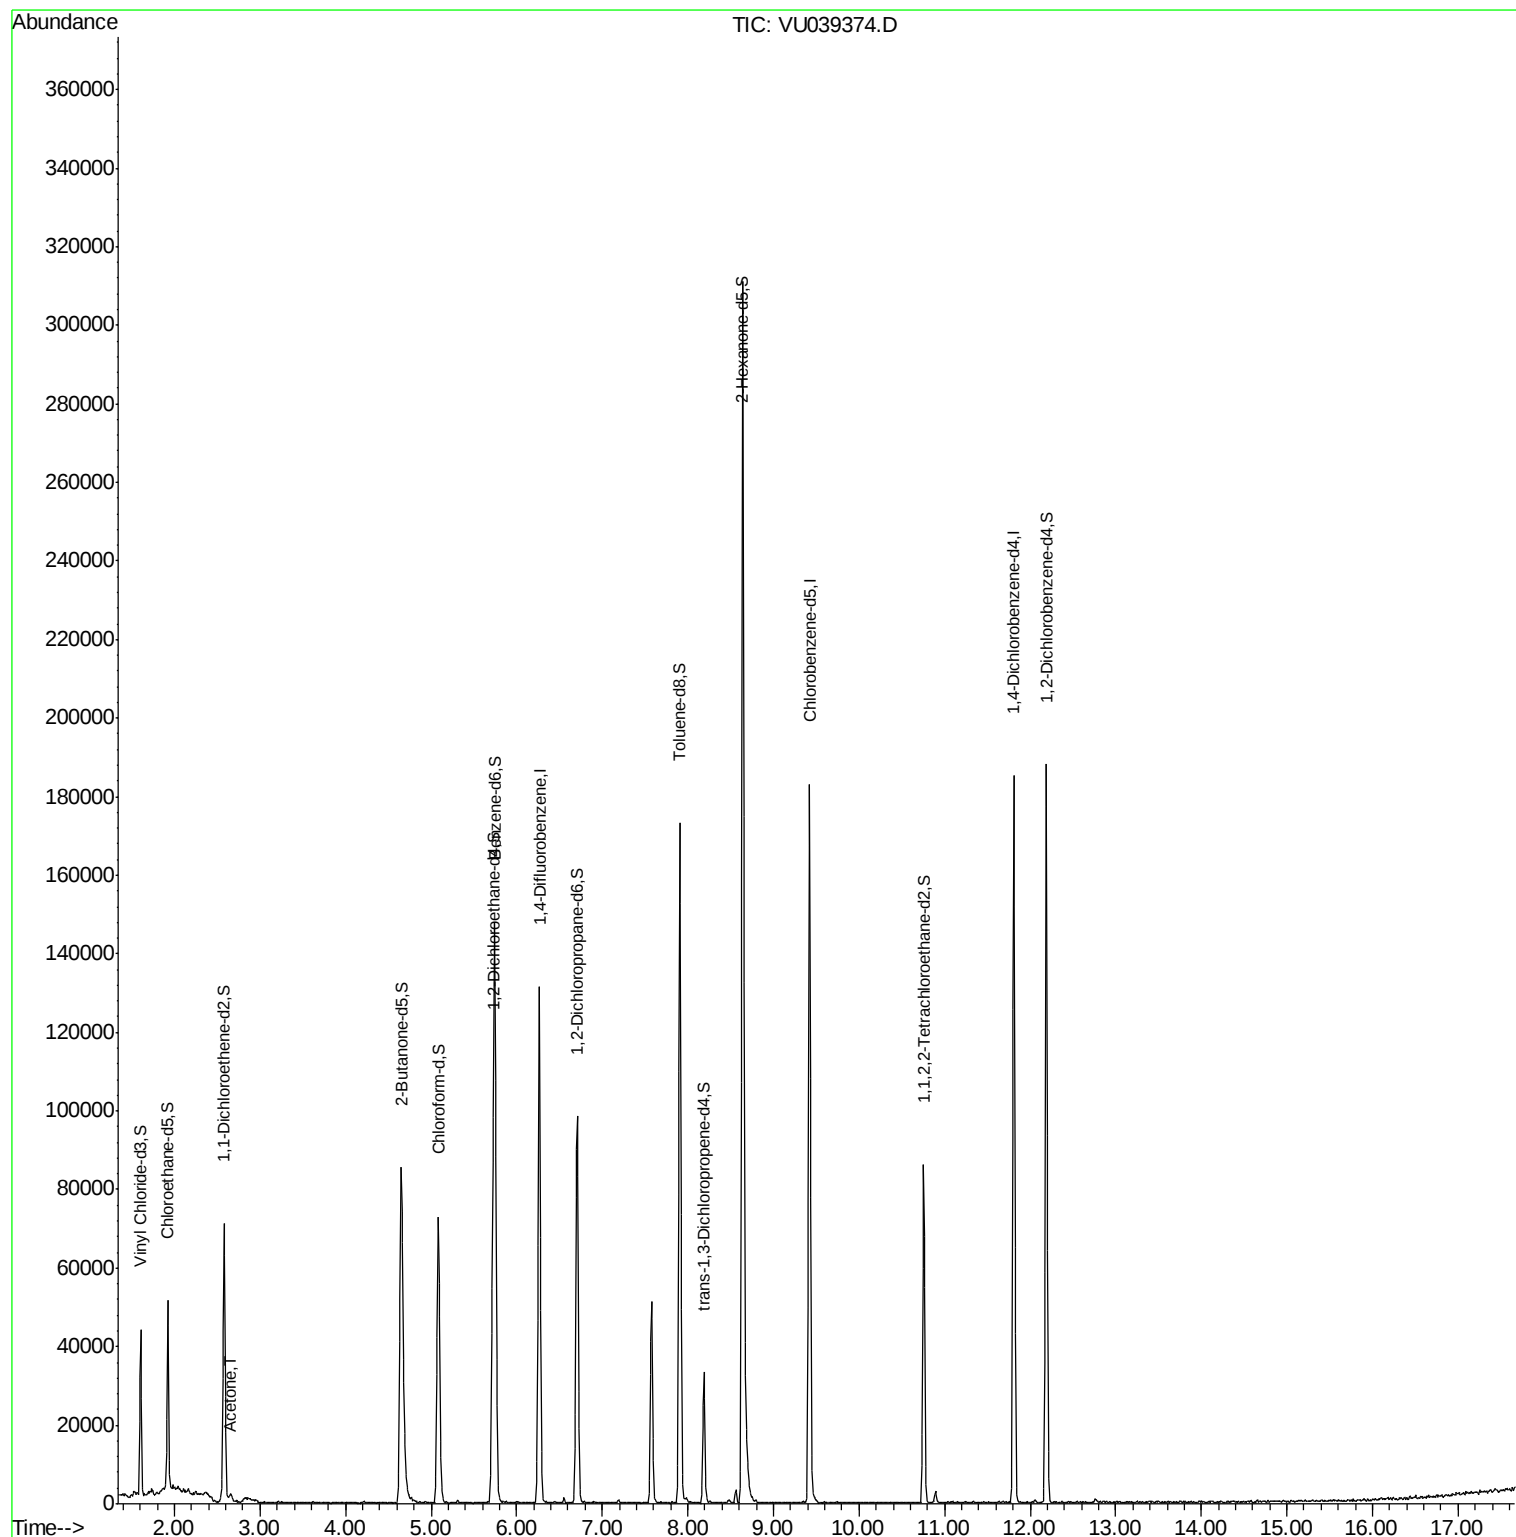

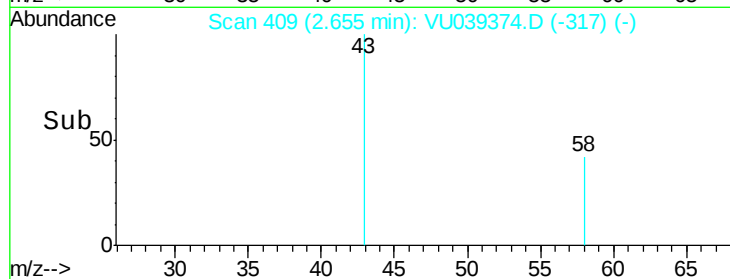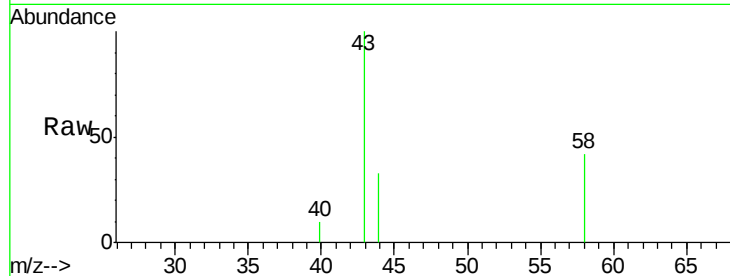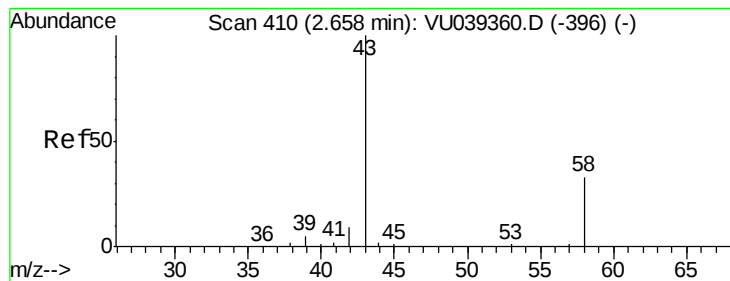

#13

Acetone

Concen: 2.577 ug/L

RT: 2.66 min Scan# 409

Delta R.T. -0.00 min

Lab File: VU039374.D

Acq: 09 Jul 2020 02:44

Instrument :
MSVOA_U
ClientSampleId :
F4A85

Tot Ion: 43 Resp: 3776

Ion Ratio Lower Upper

43 100

58 35.9 0.0 62.8

