

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070820\
 Data File : VU039379.D
 Acq On : 09 Jul 2020 04:39
 Operator : SY/MD
 Sample : L3244-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A99

Quant Time: Jul 10 09:29:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 09 05:48:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	98290	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	90626	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	44343	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	28309	4.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.40%
7) Chloroethane-d5	1.93	69	30540	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.80%
11) 1,1-Dichloroethene-d2	2.58	63	43365	3.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.40%
20) 2-Butanone-d5	4.66	46	150481	57.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.46%
24) Chloroform-d	5.09	84	65917	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.60%
26) 1,2-Dichloroethane-d4	5.72	65	44150	5.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.00%
32) Benzene-d6	5.75	84	130729	5.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	119.80%
36) 1,2-Dichloropropane-d6	6.70	67	45906	5.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	119.80%
41) Toluene-d8	7.91	98	116386	6.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.00%
43) trans-1,3-Dichloropropene-	8.19	79	17684	5.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.40%
46) 2-Hexanone-d5	8.64	63	111585	55.57	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.14%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	42631	5.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	45588	5.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.20%


Target Compounds					Ovalue
13) Acetone	2.66	43	4287	3.047 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU070820\
Data File : VU039379.D
Acq On : 09 Jul 2020 04:39
Operator : SY/MD
Sample : L3244-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A99

Quant Time: Jul 10 09:29:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 09 05:48:41 2020
Response via : Initial Calibration

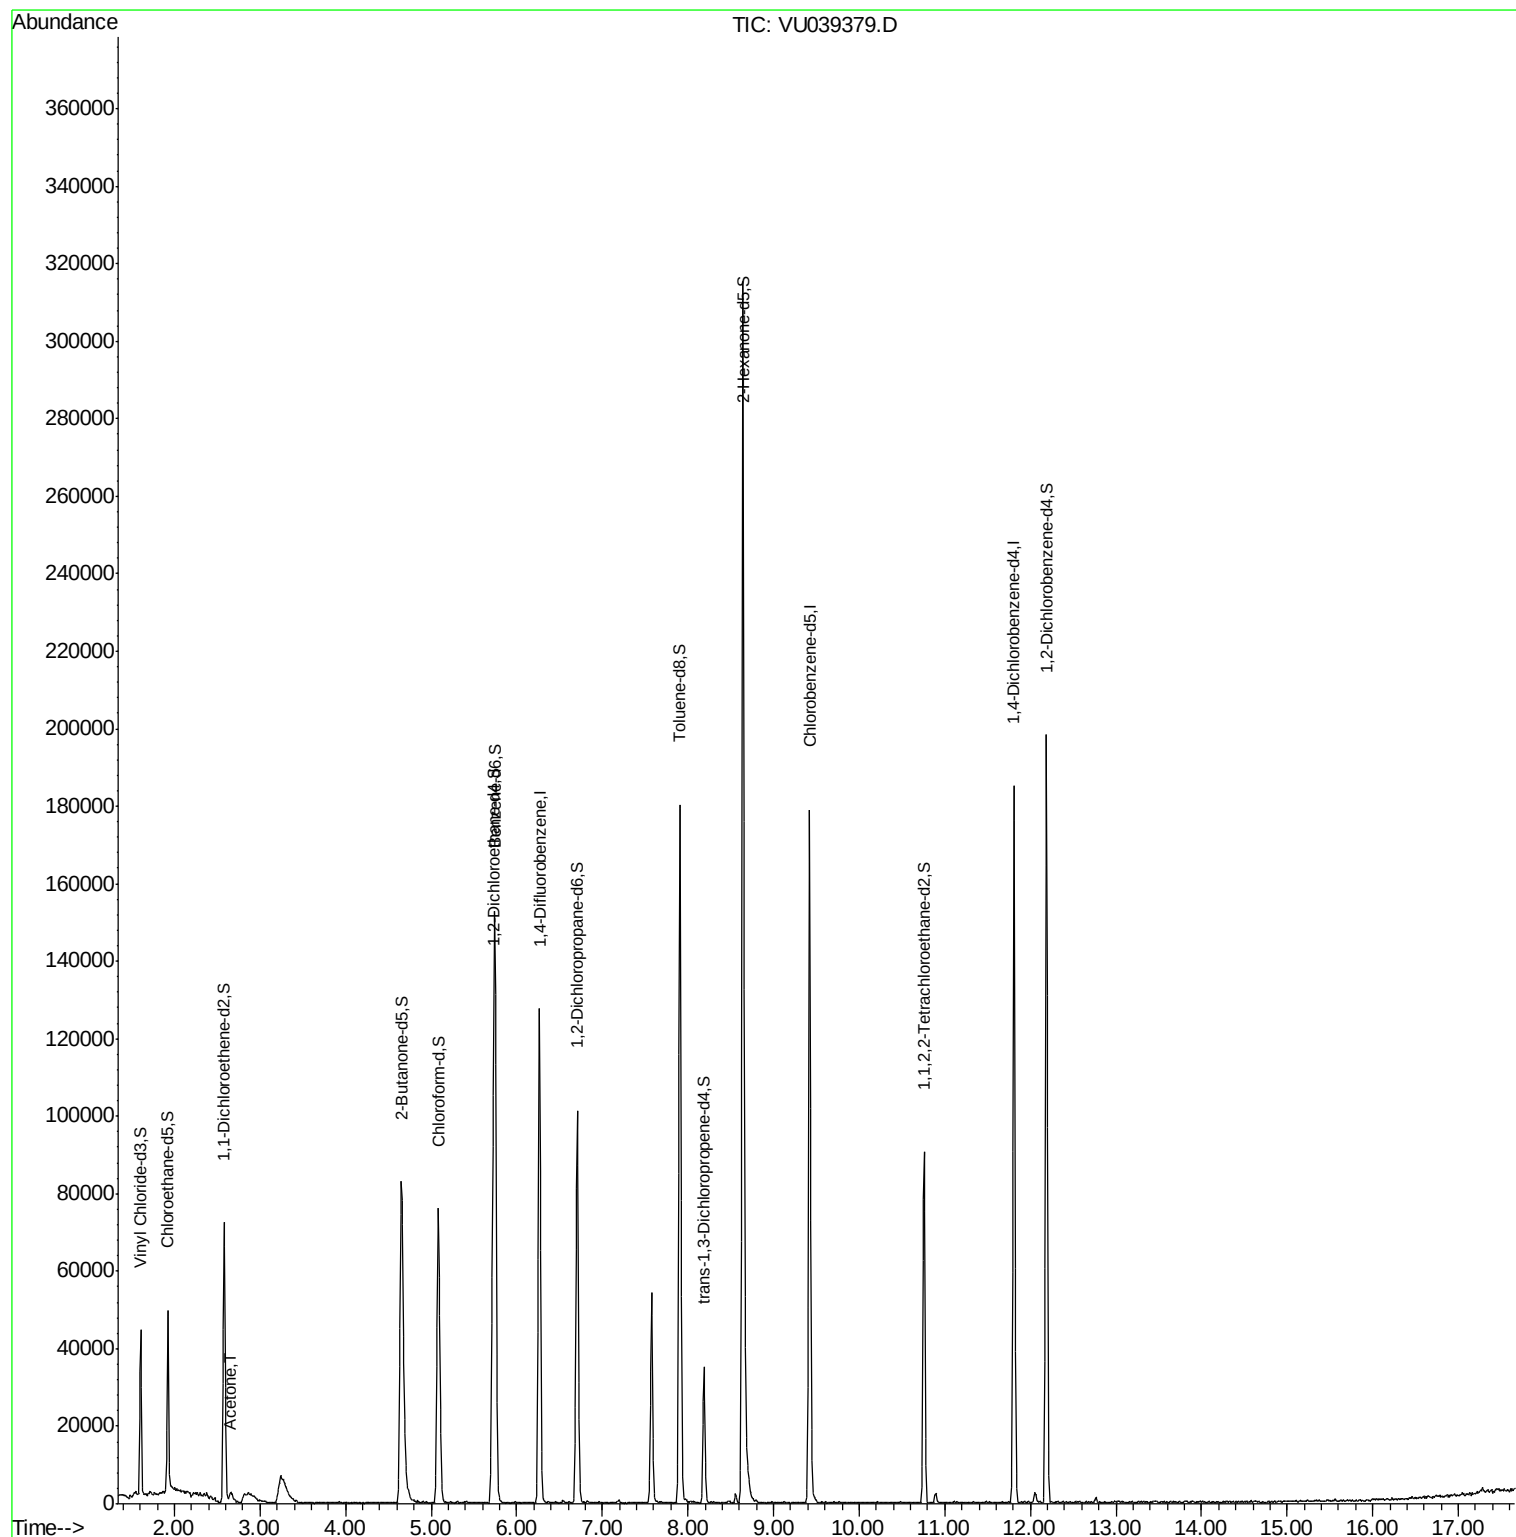

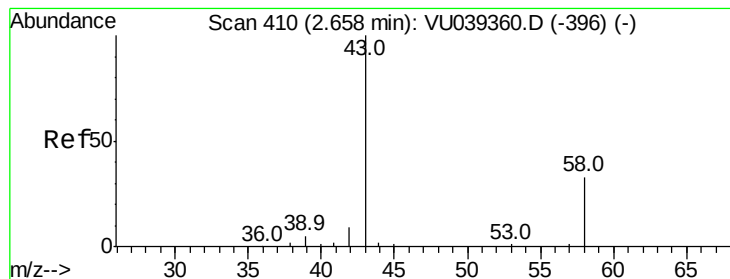

#13

Acetone

Concen: 3.047 ug/L

RT: 2.66 min Scan# 409

Delta R.T. -0.00 min

Lab File: VU039379.D

Acq: 09 Jul 2020 04:39

Instrument :
MSVOA_U
ClientSampleId :
F4A99

Tot Ion: 43 Resp: 4287

Ion Ratio Lower Upper

43 100

58 27.1 0.0 62.8

