


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070820\
 Data File : VU039340.D
 Acq On : 08 Jul 2020 08:38
 Operator : SY/MD
 Sample : BFB27
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB27

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 09 05:48:41 2020

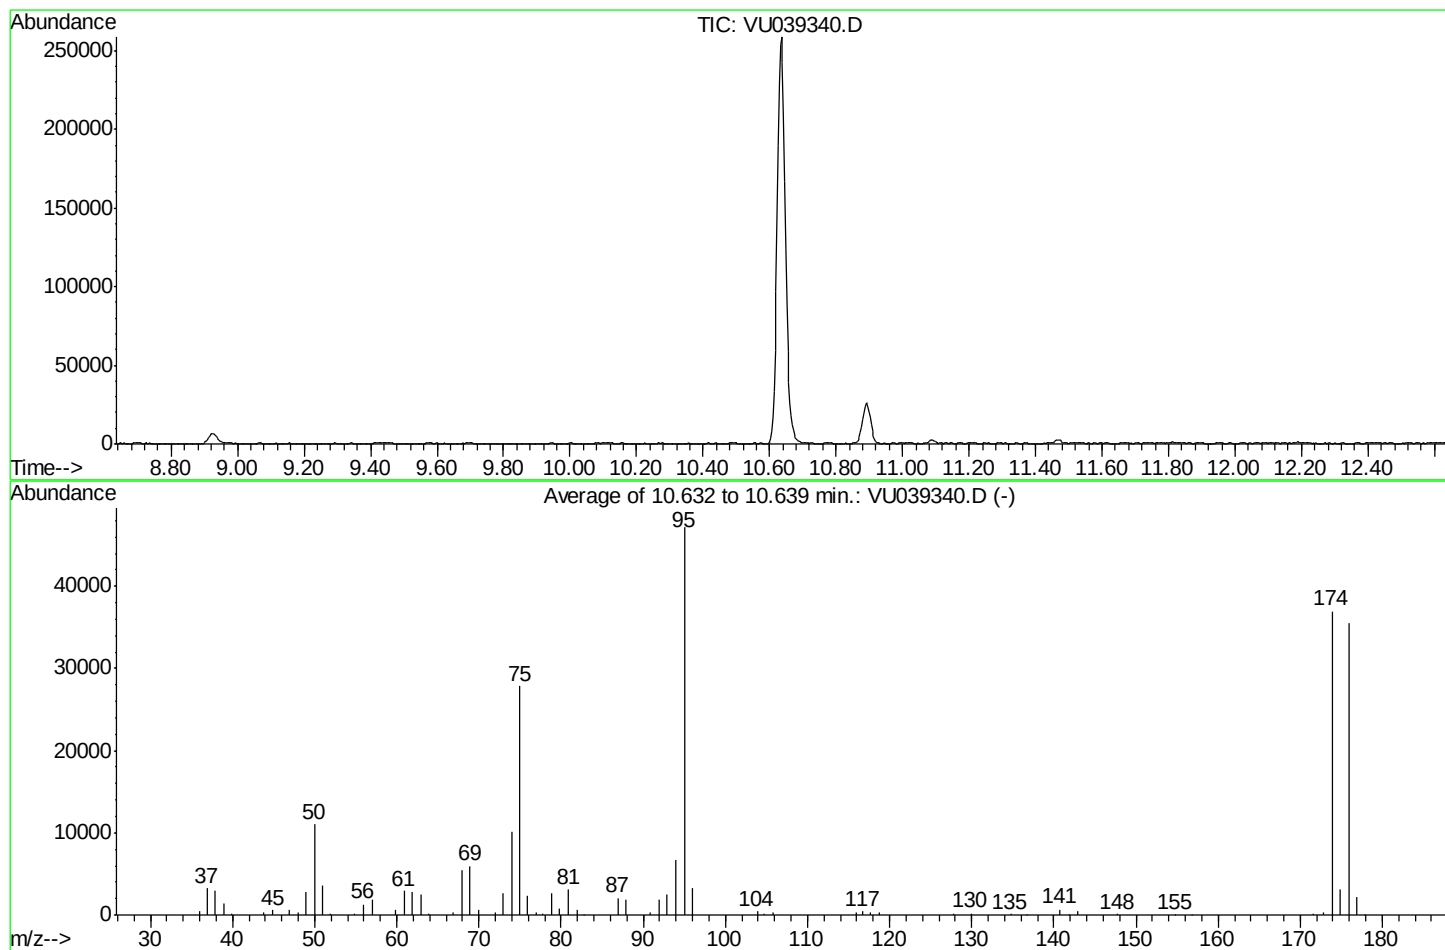

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	10988	PASS
75	95	30	80	59.1	27864	PASS
95	95	100	100	100.0	47173	PASS
96	95	5	9	7.0	3308	PASS
173	174	0.00	2	1.0	386	PASS
174	95	50	120	78.3	36917	PASS
175	174	5	9	8.3	3075	PASS
176	174	95	101	96.0	35442	PASS
177	176	5	9	6.1	2156	PASS

m/z	Abundance
35.90	477.0
36.90	3129.0
37.90	3071.0
38.90	1341.0
39.80	124.0
43.90	741.0
44.90	566.0
46.90	647.0
48.00	416.0
48.90	2710.0
50.00	11354.0
51.00	3766.0
51.90	210.0
54.90	218.0
55.90	1436.0
57.00	1909.0
59.90	625.0
60.90	2889.0
61.90	2970.0
63.00	2410.0
63.90	227.0
66.80	224.0
68.00	5915.0
68.90	6213.0
69.90	643.0
72.00	299.0
72.90	2804.0
74.00	9892.0
75.00	28224.0
75.90	2459.0
76.90	270.0
77.80	180.0
78.80	2768.0
79.80	738.0
80.90	3162.0
81.90	630.0
86.90	1928.0
87.90	1733.0
90.80	249.0
91.90	1831.0
92.90	2454.0
94.00	6901.0
95.00	47856.0
96.00	3338.0
103.90	458.0
104.70	119.0
105.80	301.0
115.90	300.0
116.80	475.0
117.70	306.0
118.70	272.0
127.80	186.0
129.90	209.0
134.70	123.0
136.70	135.0
140.80	705.0
142.90	505.0
147.80	133.0
154.80	134.0
156.70	104.0
171.70	132.0
172.90	409.0
173.90	36752.0
174.90	3106.0
175.90	34816.0
176.90	2128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.90	498.0
36.90	3327.0
37.90	3045.0
39.00	1415.0
39.80	164.0
43.90	703.0
44.90	567.0
46.90	771.0
48.00	341.0
48.90	2847.0
50.00	11302.0
51.00	3551.0
51.80	219.0
54.90	189.0
55.90	1415.0
57.00	1932.0
59.90	638.0
60.90	3003.0
61.90	2809.0
63.00	2560.0
63.90	220.0
66.80	252.0
68.00	5674.0
68.90	6062.0
69.90	630.0
72.00	260.0
72.90	2651.0
74.00	10351.0
75.00	28752.0
75.90	2428.0
76.90	341.0
77.80	242.0
78.90	2661.0
79.80	726.0
80.90	3175.0
81.90	607.0
82.80	104.0
86.90	2138.0
87.90	1925.0
90.90	276.0
91.90	1886.0
92.90	2674.0
94.00	7004.0
95.00	48504.0
96.00	3456.0
103.90	433.0
104.80	121.0
105.70	271.0
115.90	307.0
116.80	421.0
117.70	262.0
118.80	312.0
127.80	155.0
129.90	240.0
134.70	126.0
136.70	111.0
140.80	625.0
141.80	103.0
142.90	537.0
147.80	156.0
154.80	114.0
171.60	133.0
172.90	384.0
173.90	37960.0
174.90	3172.0
175.90	36256.0
176.90	2192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.90	490.0
36.90	3215.0
37.90	2750.0
39.00	1325.0
39.80	190.0
43.80	768.0
44.90	571.0
46.90	686.0
47.80	261.0
48.90	2666.0
50.00	10309.0
50.90	3262.0
51.80	184.0
54.90	167.0
55.90	1134.0
56.90	1853.0
59.90	546.0
60.90	2940.0
61.90	2507.0
63.00	2350.0
63.90	185.0
66.90	249.0
68.00	5009.0
68.90	5632.0
69.90	554.0
72.10	192.0
72.90	2293.0
74.00	10007.0
75.00	26616.0
75.90	2107.0
76.90	391.0
77.80	233.0
78.90	2520.0
79.80	682.0
80.90	2806.0
81.90	566.0
86.90	2169.0
87.90	1877.0
90.90	284.0
91.90	1691.0
92.90	2582.0
94.00	6428.0
95.00	45160.0
96.00	3131.0
103.90	351.0
104.80	118.0
105.70	232.0
115.90	296.0
116.70	375.0
117.70	179.0
118.80	333.0
127.80	174.0
129.90	216.0
134.80	107.0
140.70	552.0
142.90	560.0
147.80	149.0
171.50	113.0
172.90	365.0
173.90	36040.0
174.90	2948.0
175.90	35256.0
176.90	2148.0
177.80	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
43.80	401.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27