

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070821\
 Data File : VU044327.D
 Acq On : 08 Jul 2021 17:00
 Operator : SY/MD
 Sample : VU0708WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0708WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044327.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.057	524	534	544	rVB3	5652	10436	15.61%	4.802%
2	3.150	555	563	564	rBV4	808	1163	1.74%	0.535%
3	3.726	740	742	751	rVB5	718	748	1.12%	0.344%
4	4.694	1035	1043	1054	rBV4	3807	9376	14.03%	4.314%
5	6.121	1474	1487	1503	rBV	31590	61682	92.27%	28.384%
6	7.902	2034	2041	2048	rBV4	455	708	1.06%	0.326%
7	10.642	2883	2893	2905	rBV2	31060	50953	76.22%	23.447%
8	11.105	3030	3037	3043	rVB3	532	713	1.07%	0.328%
9	11.754	3233	3239	3246	rBV3	550	693	1.04%	0.319%
10	11.848	3264	3268	3273	rVB3	1029	905	1.35%	0.416%
11	12.201	3365	3378	3395	rBV	39768	66849	100.00%	30.761%
12	13.848	3884	3890	3899	rVB4	2197	3175	4.75%	1.461%
13	14.095	3958	3967	3981	rBV2	3866	6471	9.68%	2.978%
14	14.343	4036	4044	4051	rVB5	2380	3443	5.15%	1.584%


Sum of corrected areas: 217315

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070821\
Data File : VU044327.D
Acq On : 08 Jul 2021 17:00
Operator : SY/MD
Sample : VU0708WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

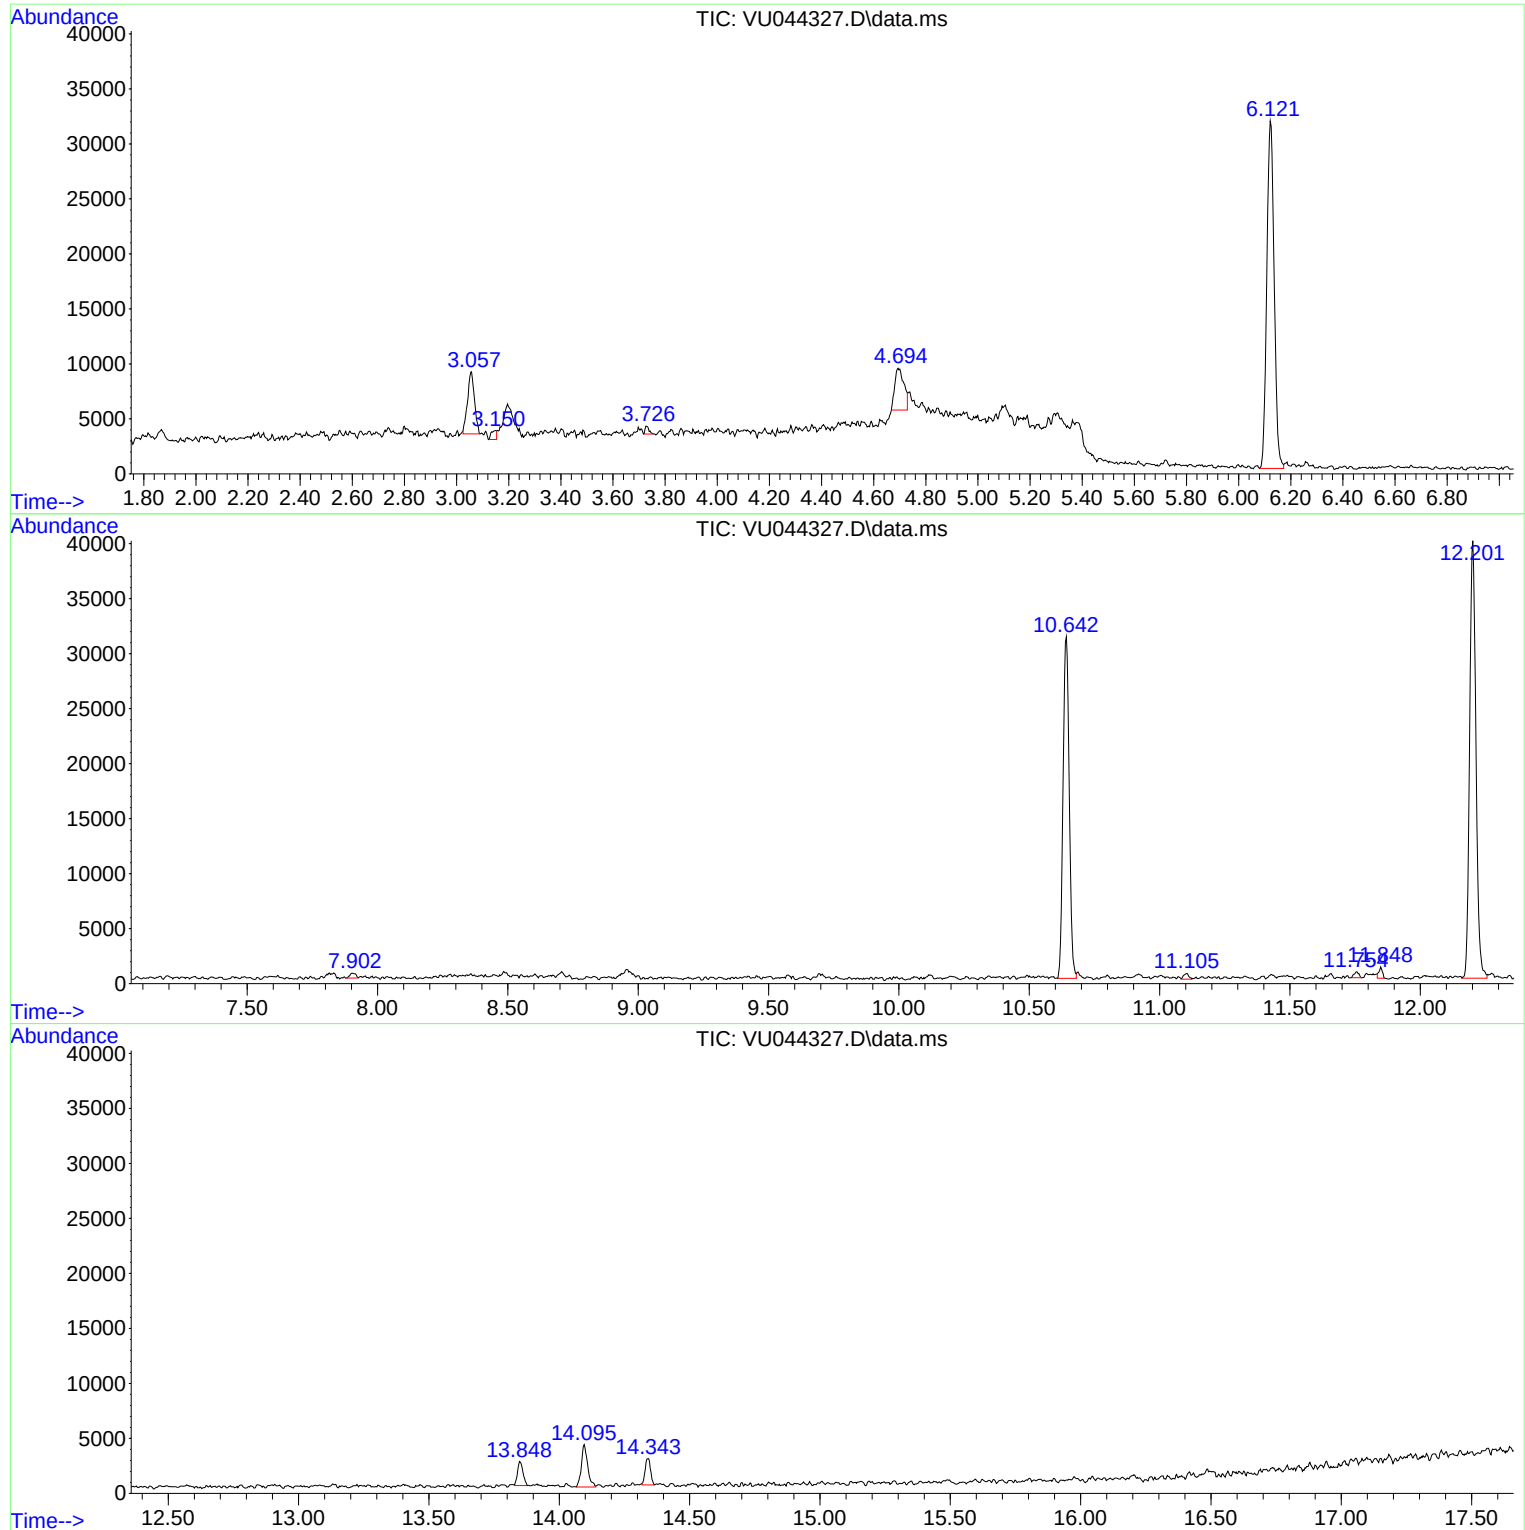

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070821\
Data File : VU044327.D
Acq On : 08 Jul 2021 17:00
Operator : SY/MD
Sample : VU0708WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070821\
Data File : VU044327.D
Acq On : 08 Jul 2021 17:00
Operator : SY/MD
Sample : VU0708WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
