
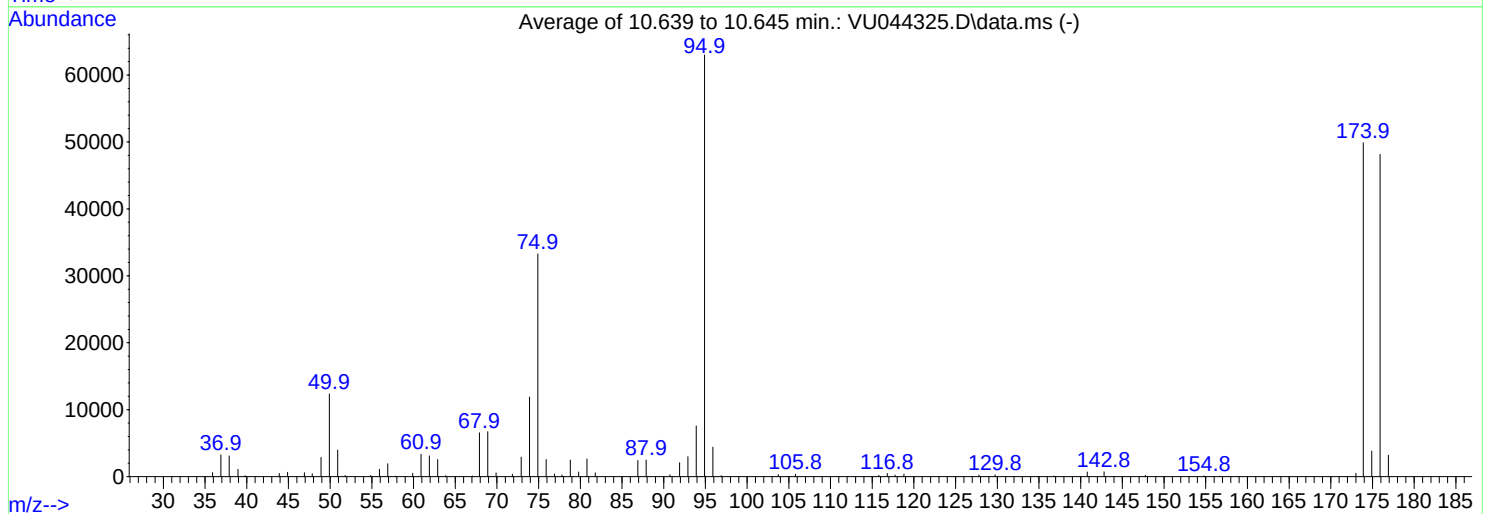


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070821\
Data File : VU044325.D
Acq On : 08 Jul 2021 15:38
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070721DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jul 08 15:34:52 2021

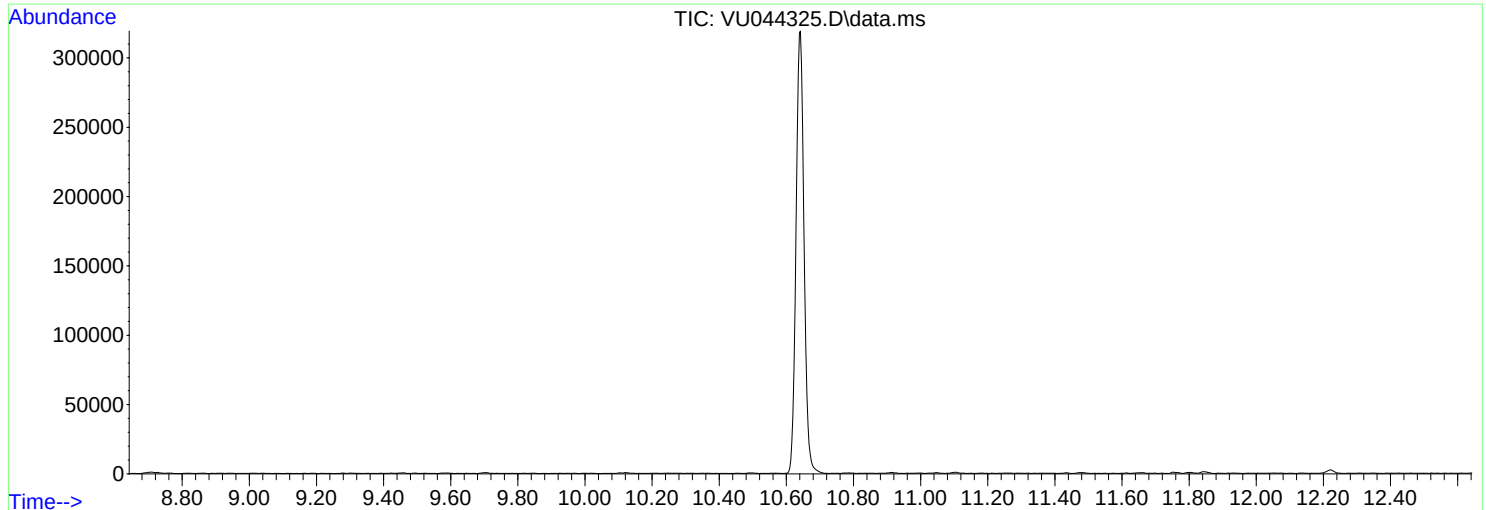

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	12355	PASS
75	95	30	60	52.8	33267	PASS
95	95	100	100	100.0	63016	PASS
96	95	5	9	7.0	4406	PASS
173	174	0.00	2	1.0	493	PASS
174	95	50	100	79.2	49899	PASS
175	174	5	9	7.7	3821	PASS
176	174	95	101	96.5	48152	PASS
177	176	5	9	6.6	3196	PASS