

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070822\
 Data File : VU049658.D
 Acq On : 08 Jul 2022 15:48
 Operator : SY/MD
 Sample : VU0708WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0708WBL01

Quant Time: Jul 09 04:37:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 07 07:00:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.115	96	34548	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	11384	0.900	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	11515	0.988	ug/l	0.00
Spiked Amount 1.000			Recovery	=	99.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070822\
Data File : VU049658.D
Acq On : 08 Jul 2022 15:48
Operator : SY/MD
Sample : VU0708WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01

Quant Time: Jul 09 04:37:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 07 07:00:33 2022
Response via : Initial Calibration




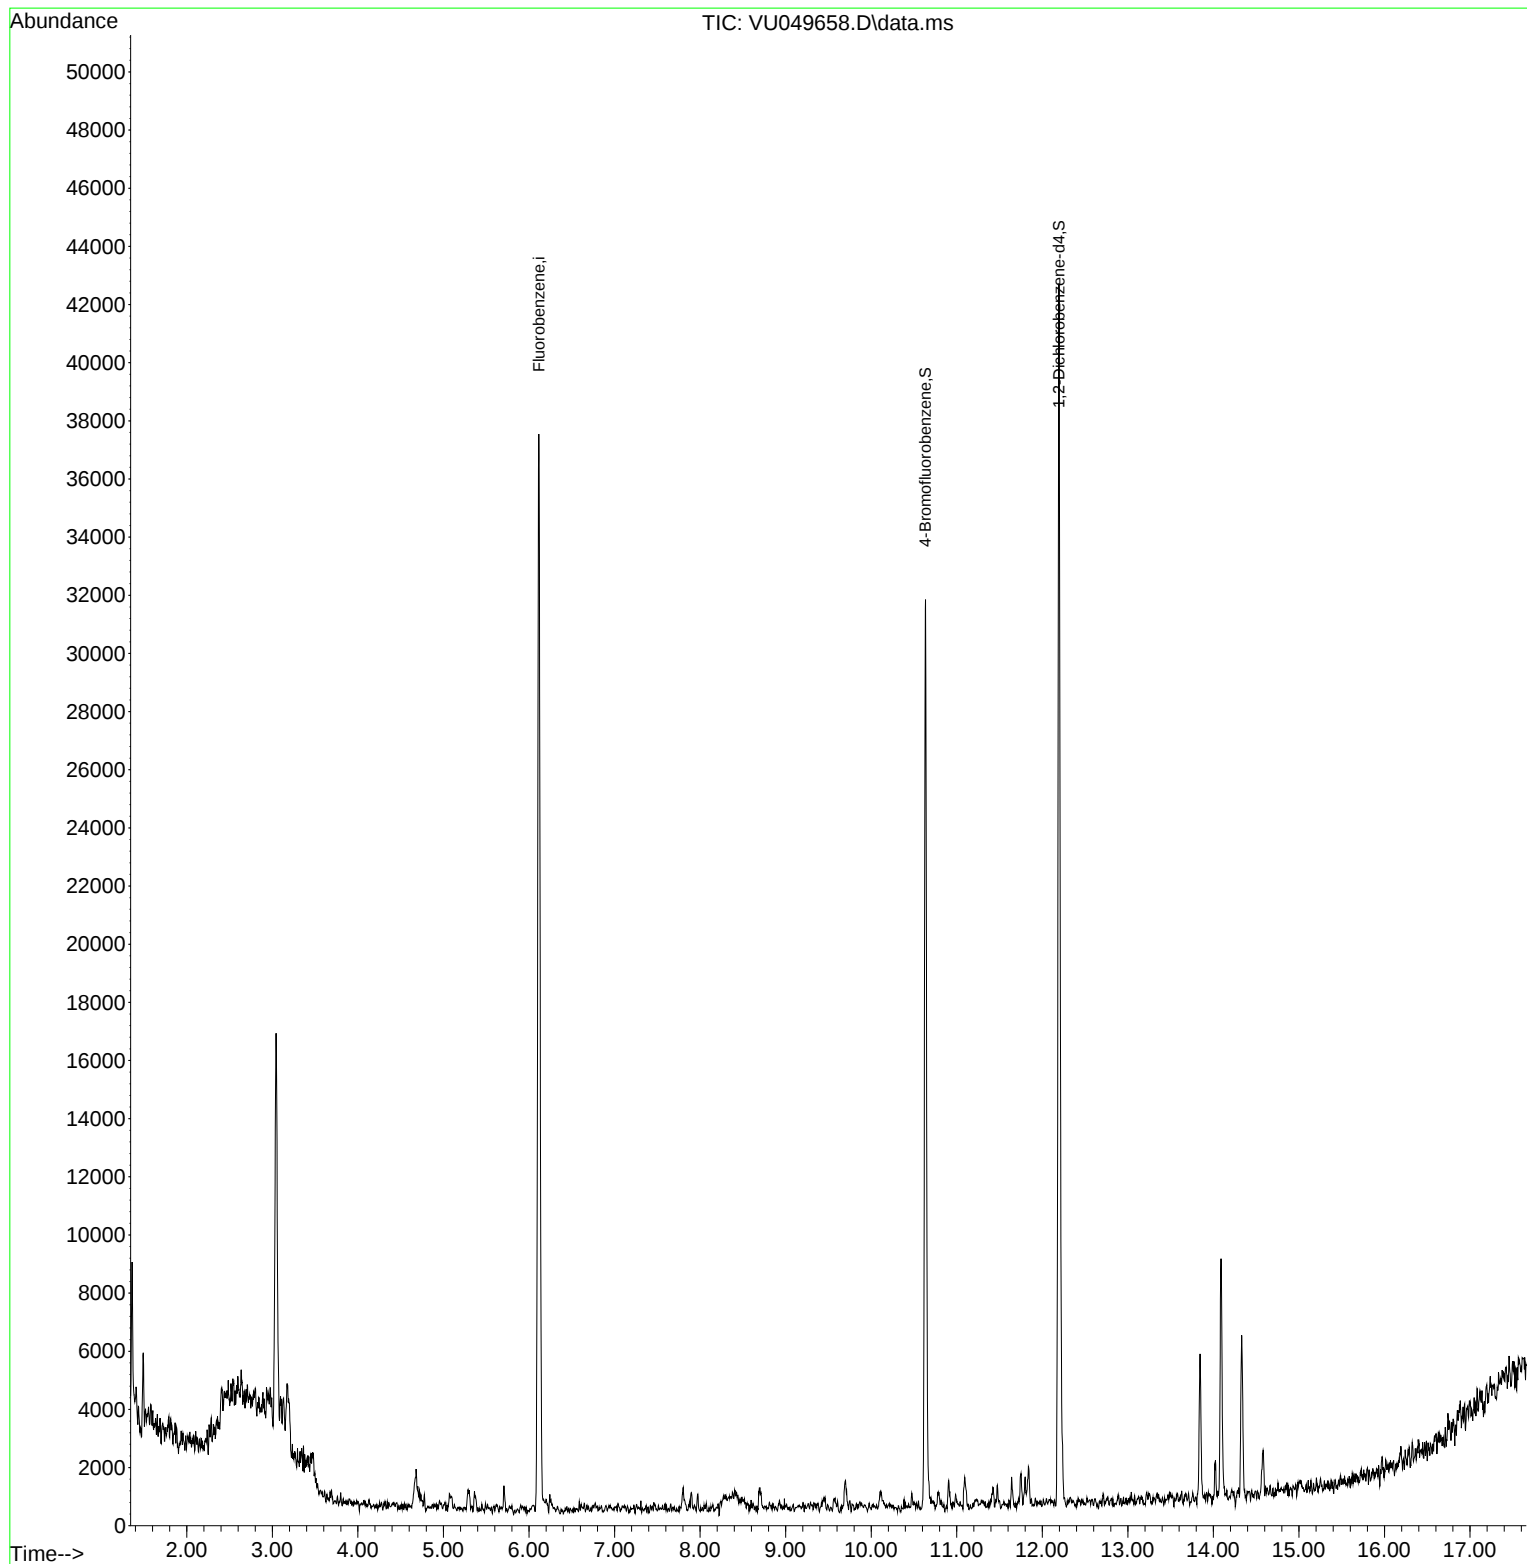


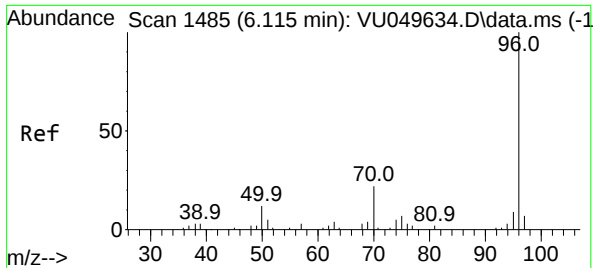

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1485
Delta R.T. -0.000 min
Lab File: VU049658.D
Acq: 08 Jul 2022 15:48




Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01


Tgt Ion: 96	Resp: 34548
Ion Ratio	Lower Upper
96 100	
70 20.3	16.7 25.1
95 8.8	7.4 11.0
97 6.4	0.0 0.0

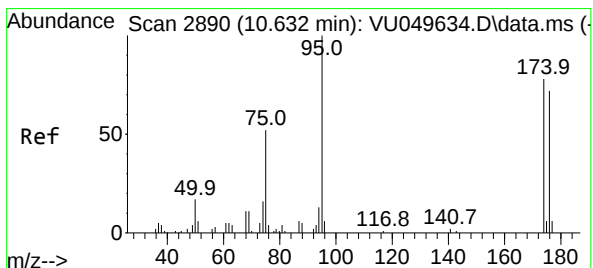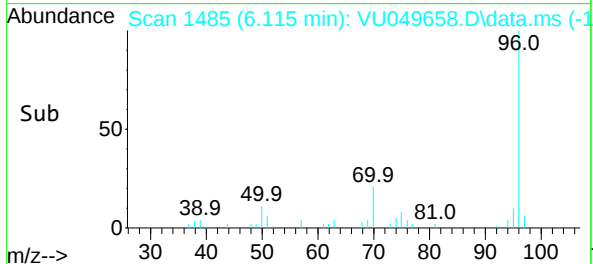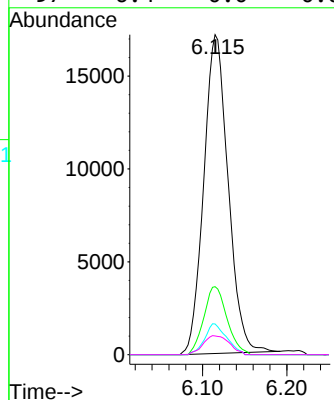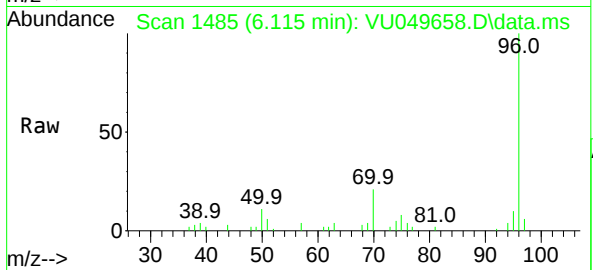

#57
4-Bromofluorobenzene
Concen: 0.900 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. 0.000 min
Lab File: VU049658.D
Acq: 08 Jul 2022 15:48


Tgt Ion: 95	Resp: 11384
Ion Ratio	Lower Upper
95 100	
174 77.1	62.4 93.6
176 76.0	56.2 84.2

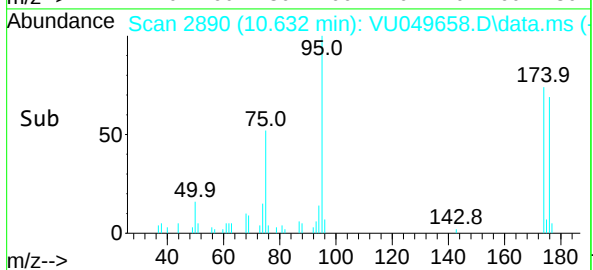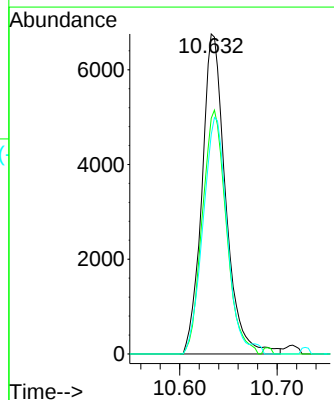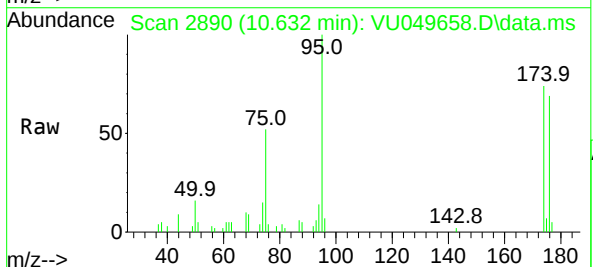

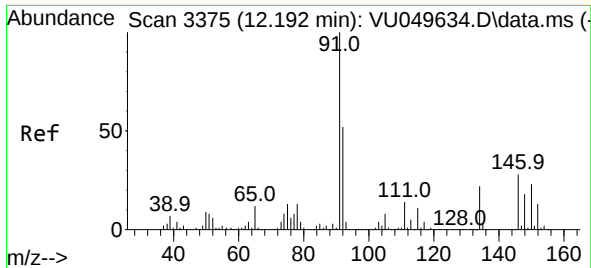

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.988 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU049658.D
 Acq: 08 Jul 2022 15:48

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0708WBL01

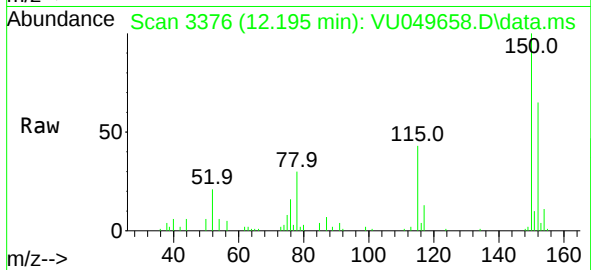

Tgt Ion:	152	Resp:	11515
Ion	Ratio	Lower	Upper
152	100		
115	64.6	0.0	254.6
150	157.4	0.0	623.6

