

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070822\
 Data File : VU049658.D
 Acq On : 08 Jul 2022 15:48
 Operator : SY/MD
 Sample : VU0708WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0708WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU049658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.404	326	331	332	rBV2	1169	986	1.32%	0.348%
2	2.932	493	495	500	rBV4	886	843	1.13%	0.298%
3	3.044	519	530	542	rBV2	13525	25437	34.06%	8.977%
4	3.131	552	557	563	rVB5	1119	1393	1.87%	0.492%
5	3.173	563	570	574	rBV6	1619	2320	3.11%	0.819%
6	4.681	1025	1039	1044	rBV2	1190	2241	3.00%	0.791%
7	5.289	1221	1228	1230	rBV4	689	811	1.09%	0.286%
8	5.707	1353	1358	1365	rVB3	881	944	1.26%	0.333%
9	6.115	1472	1485	1501	rBV	37055	72541	97.14%	25.602%
10	7.803	2002	2010	2013	rBV2	716	868	1.16%	0.306%
11	8.697	2280	2288	2291	rBV3	847	1221	1.64%	0.431%
12	9.700	2592	2600	2611	rVB3	1021	1932	2.59%	0.682%
13	10.636	2877	2891	2906	rBV2	31254	51136	68.48%	18.047%
14	10.906	2969	2975	2983	rBV2	978	1438	1.93%	0.508%
15	11.092	3027	3033	3043	rBV3	1103	1976	2.65%	0.697%
16	11.642	3199	3204	3211	rBV2	1051	1209	1.62%	0.427%
17	11.751	3231	3238	3244	rVB5	1084	1468	1.97%	0.518%
18	11.800	3245	3253	3258	rBV3	960	1200	1.61%	0.424%
19	11.838	3258	3265	3272	rVB4	1266	1913	2.56%	0.675%
20	12.195	3364	3376	3394	rBV2	42049	74677	100.00%	26.356%
21	13.844	3877	3889	3900	rBV6	5189	8323	11.15%	2.937%
22	14.025	3937	3945	3951	rBV3	1351	1638	2.19%	0.578%
23	14.089	3956	3965	3979	rVV2	8168	13025	17.44%	4.597%
24	14.330	4032	4040	4050	rBV3	5575	8785	11.76%	3.100%
25	14.581	4109	4118	4124	rVB3	1580	2586	3.46%	0.913%
26	16.629	4750	4755	4758	rBV4	740	797	1.07%	0.281%
27	16.851	4821	4824	4827	rBV3	866	748	1.00%	0.264%
28	17.455	5010	5012	5018	rVB5	1040	889	1.19%	0.314%




Sum of corrected areas: 283345

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070822\
Data File : VU049658.D
Acq On : 08 Jul 2022 15:48
Operator : SY/MD
Sample : VU0708WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

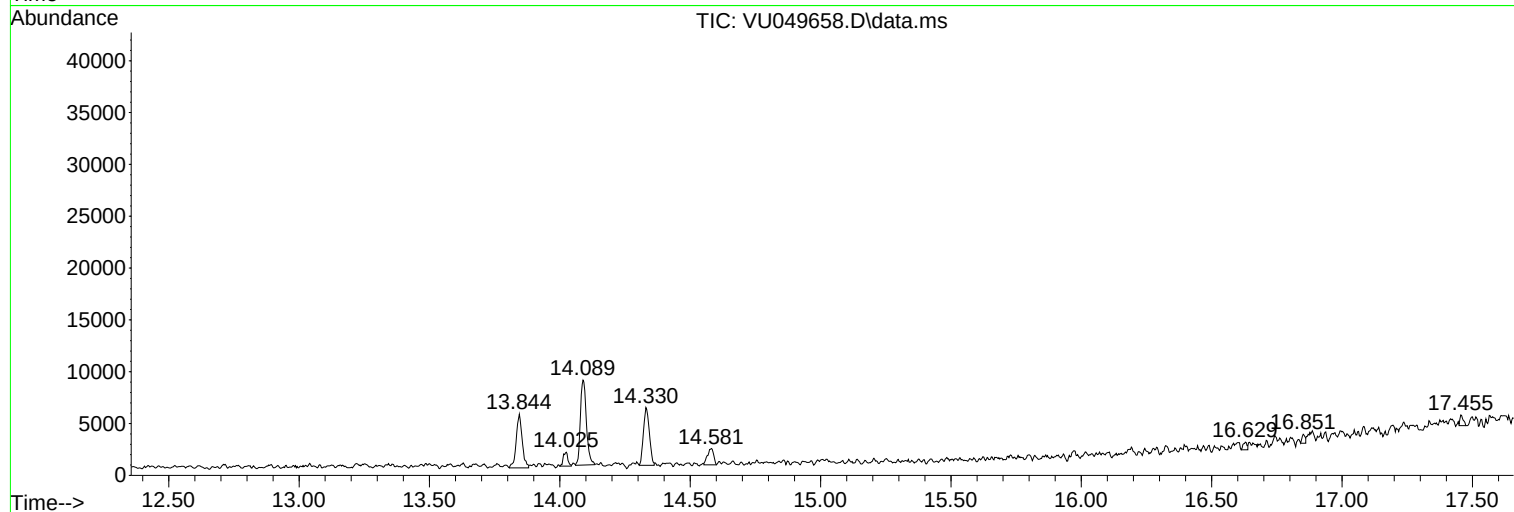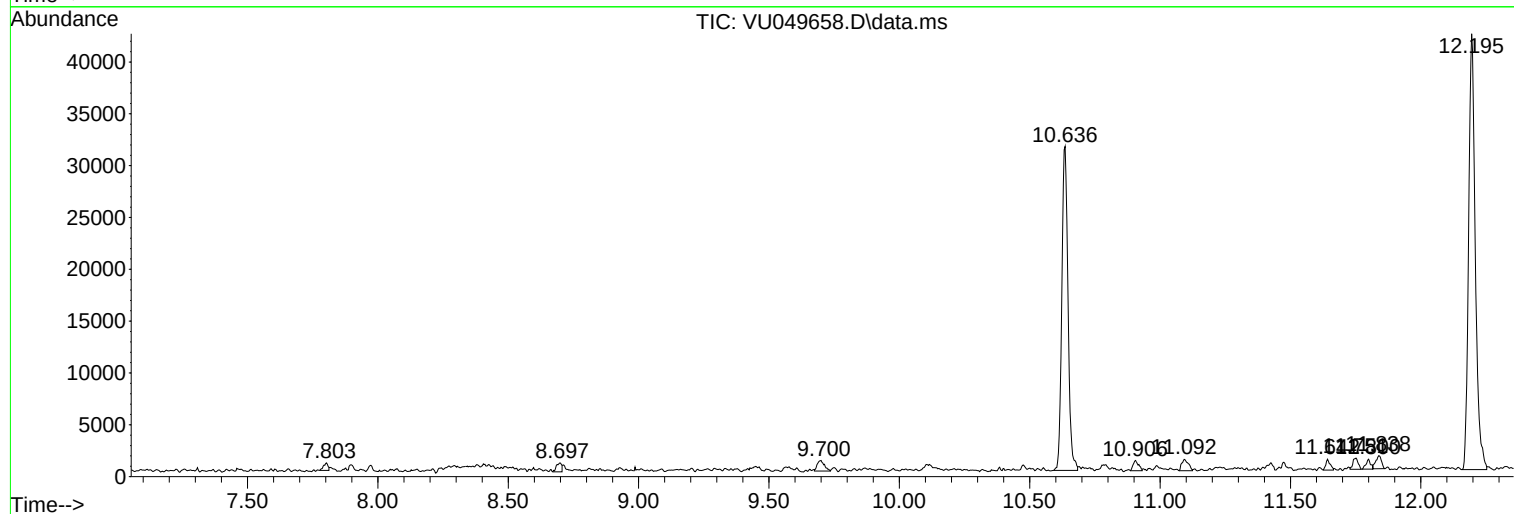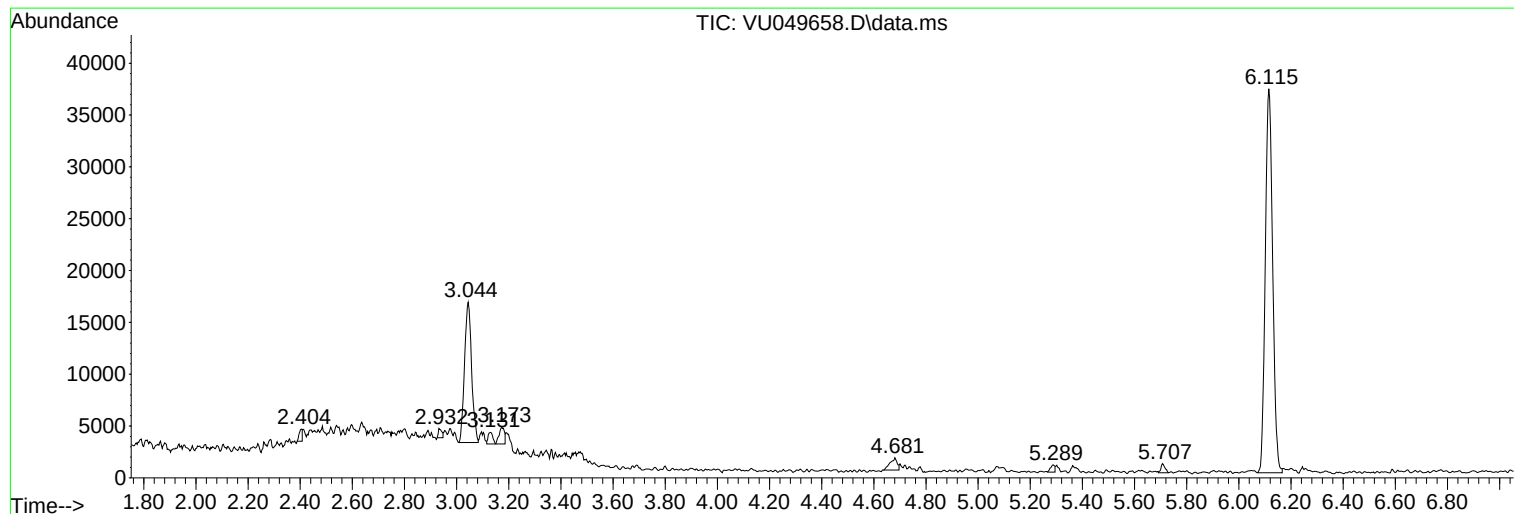

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070822\
Data File : VU049658.D
Acq On : 08 Jul 2022 15:48
Operator : SY/MD
Sample : VU0708WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070822\
Data File : VU049658.D
Acq On : 08 Jul 2022 15:48
Operator : SY/MD
Sample : VU0708WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0708WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U070622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------