

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070824\
 Data File : VU059882.D
 Acq On : 08 Jul 2024 14:46
 Operator : MD/SY
 Sample : P3138-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZN1

Quant Time: Jul 09 02:37:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 09 02:28:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	162040	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	165561	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	73980	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	44822	3.978	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.600%
7) Chloroethane-d5	1.907	69	43623	4.024	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.400%
11) 1,1-Dichloroethene-d2	2.560	65	17441	3.731	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.600%
20) 2-Butanone-d5	4.618	46	137918	59.423	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.840%
24) Chloroform-d	5.055	84	101464	4.387	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.695	65	52586	4.720	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.721	84	198693	4.361	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	6.685	67	66757	4.781	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.600%
41) Toluene-d8	7.894	98	163435	3.858	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.200%
43) trans-1,3-Dichloroprop...	8.177	79	22774	5.209	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.200%
46) 2-Hexanone-d5	8.627	63	112008	61.658	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.320%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	61244	5.309	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	69749	5.297	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%
Target Compounds						
					Qvalue	
13) Acetone	2.631	43	18189	12.081	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070824\
Data File : VU059882.D
Acq On : 08 Jul 2024 14:46
Operator : MD/SY
Sample : P3138-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZN1

Quant Time: Jul 09 02:37:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 09 02:28:04 2024
Response via : Initial Calibration

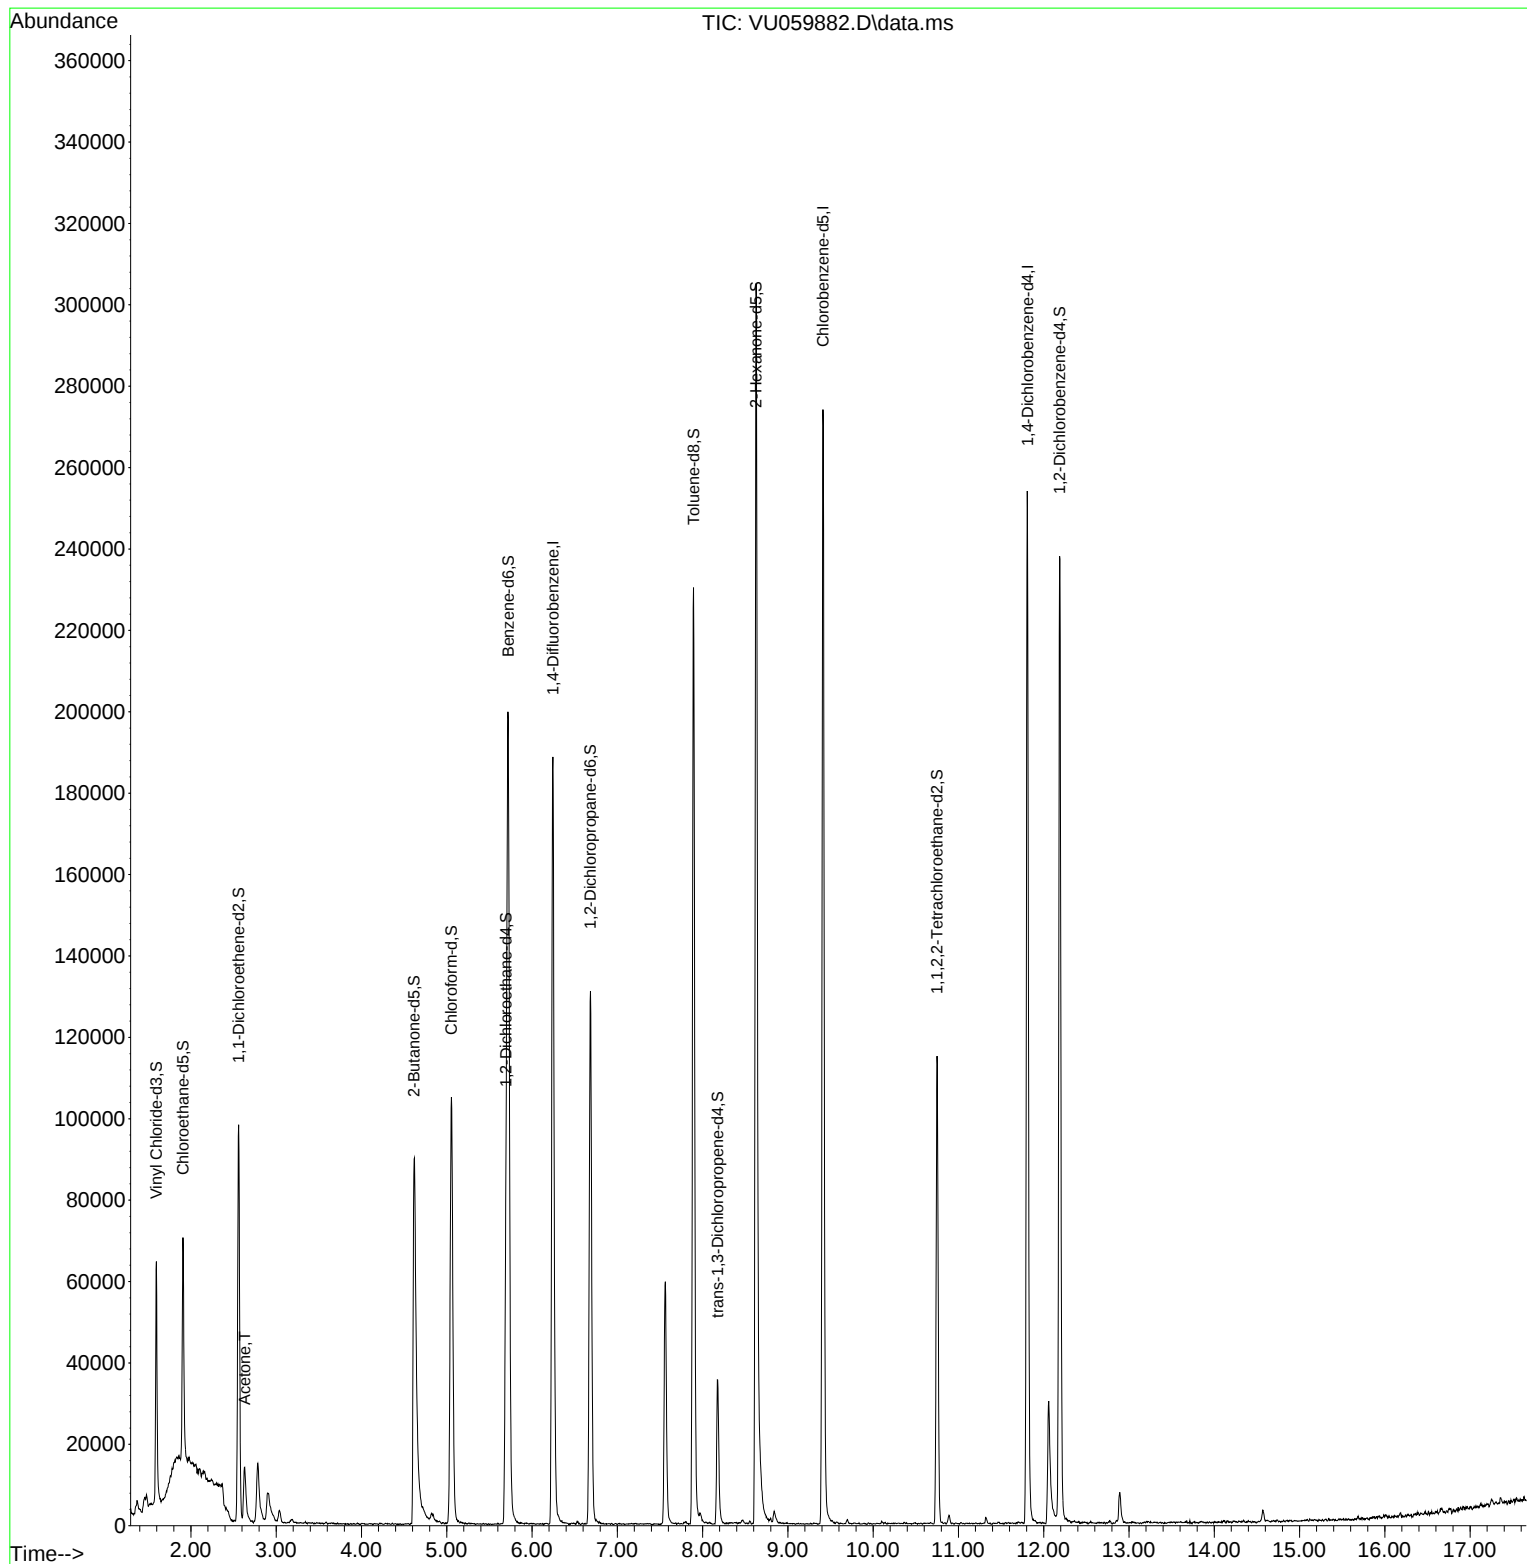

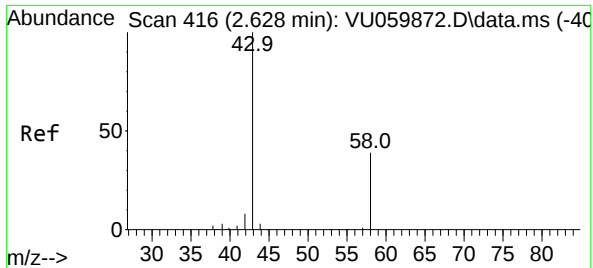

#13
 Acetone
 Concen: 12.081 ug/L
 RT: 2.631 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU059882.D
 Acq: 08 Jul 2024 14:46

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZN1

Tgt Ion: 43 Resp: 18189
 Ion Ratio Lower Upper
 43 100
 58 36.4 0.0 68.0

