

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070824\
 Data File : VU059884.D
 Acq On : 08 Jul 2024 15:33
 Operator : MD/SY
 Sample : P3137-17DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZG6DL

Quant Time: Jul 09 02:37:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 09 02:28:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	156508	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	161434	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	71916	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	43301	3.979	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.600%
7) Chloroethane-d5	1.907	69	40996	3.915	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.400%
11) 1,1-Dichloroethene-d2	2.560	65	16878	3.738	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.800%
20) 2-Butanone-d5	4.618	46	130390	58.166	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.340%
24) Chloroform-d	5.055	84	99087	4.436	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	5.695	65	50639	4.706	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	5.721	84	191008	4.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
36) 1,2-Dichloropropane-d6	6.685	67	63168	4.640	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.800%
41) Toluene-d8	7.894	98	155925	3.775	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.600%
43) trans-1,3-Dichloroprop...	8.177	79	20485	4.805	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.200%
46) 2-Hexanone-d5	8.627	63	107486	60.682	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	121.360%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	58085	5.164	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	65125	5.088	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.800%
Target Compounds						Qvalue
16) Methylene chloride	3.039	84	13109	0.997	ug/L	93
22) cis-1,2-Dichloroethene	4.660	96	74140	5.827	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070824\
Data File : VU059884.D
Acq On : 08 Jul 2024 15:33
Operator : MD/SY
Sample : P3137-17DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZG6DL

Quant Time: Jul 09 02:37:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 09 02:28:04 2024
Response via : Initial Calibration




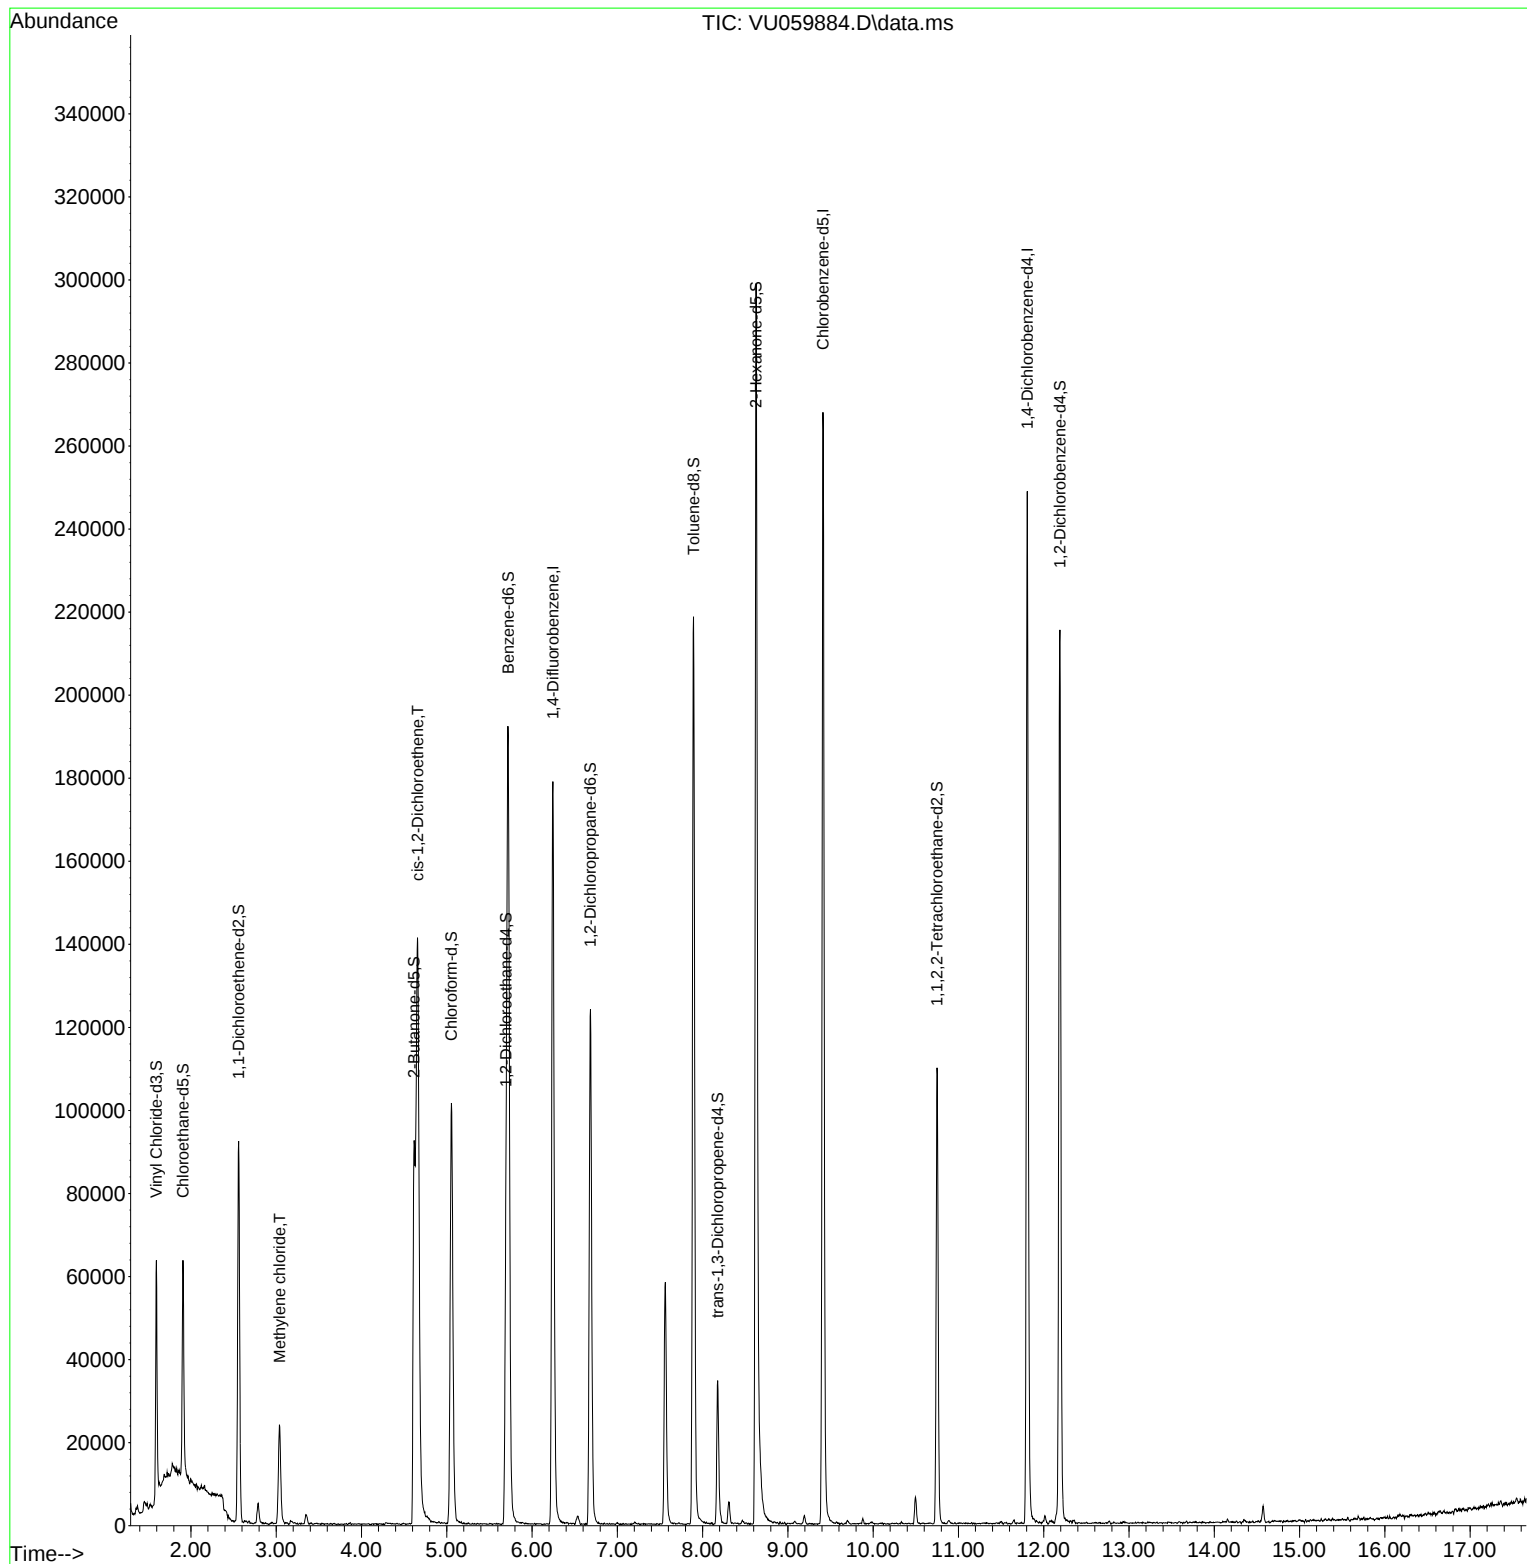


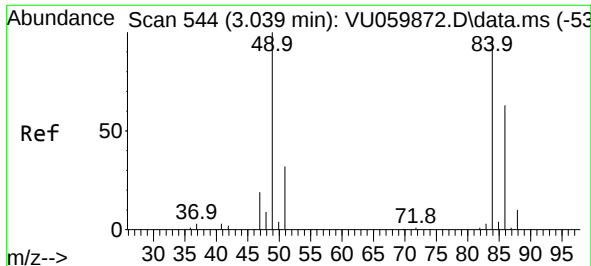

#16
Methylene chloride
Concen: 0.997 ug/L
RT: 3.039 min Scan# 544
Delta R.T. 0.000 min
Lab File: VU059884.D
Acq: 08 Jul 2024 15:33

Instrument :
MSVOA_U
ClientSampleId :
YDZG6DL

Tgt Ion: 84 Resp: 13109
Ion Ratio Lower Upper
84 100
86 66.0 42.1 78.1
49 107.8 80.6 149.8

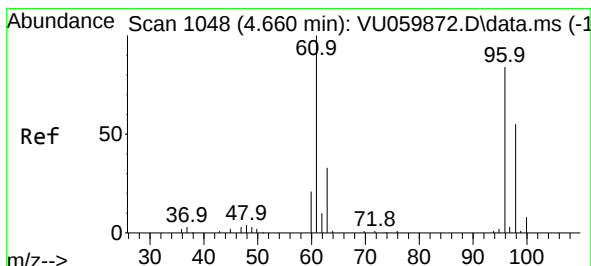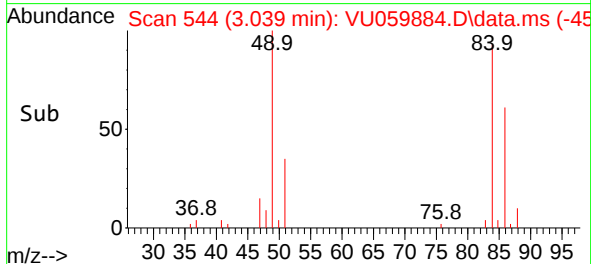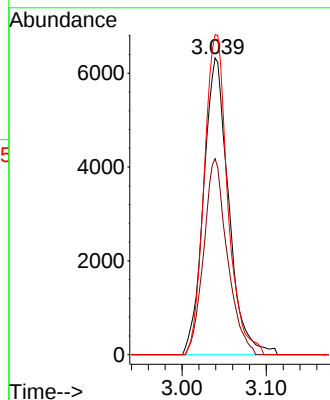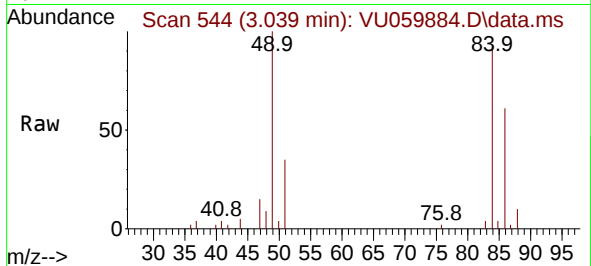

#22
cis-1,2-Dichloroethene
Concen: 5.827 ug/L
RT: 4.660 min Scan# 1048
Delta R.T. 0.000 min
Lab File: VU059884.D
Acq: 08 Jul 2024 15:33

Tgt Ion: 96 Resp: 74140
Ion Ratio Lower Upper
96 100
61 115.9 87.4 162.2
98 62.9 42.3 78.5

