
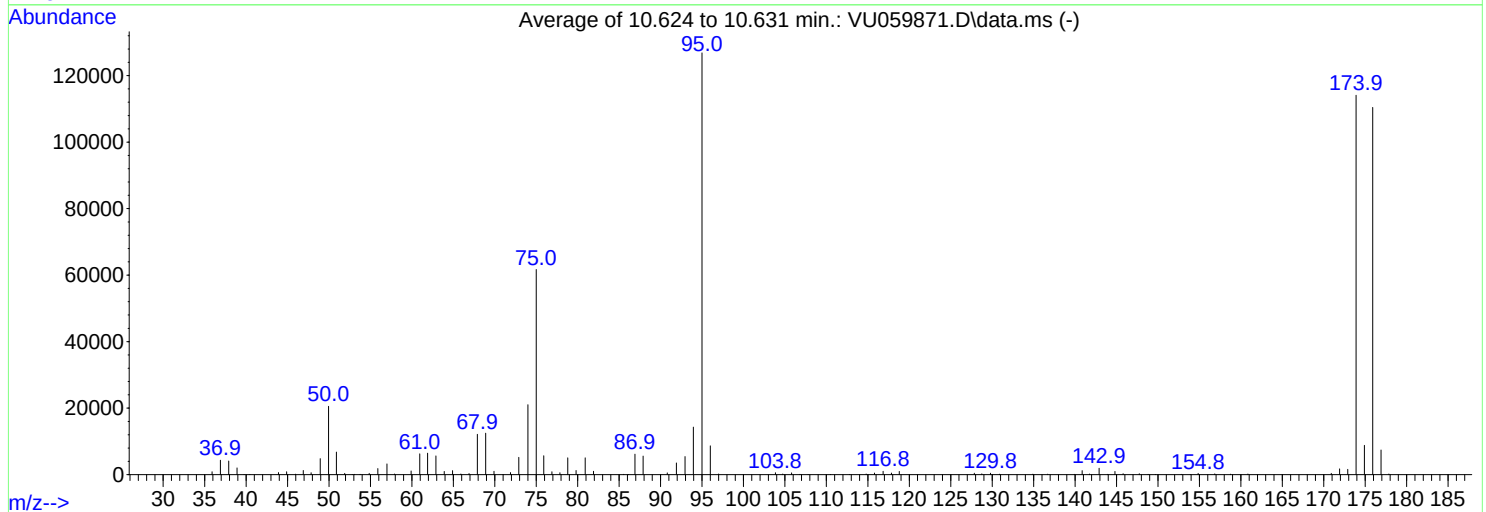


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070824\
Data File : VU059871.D
Acq On : 08 Jul 2024 08:59
Operator : MD/SY
Sample : BFB171
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB171

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jul 09 02:28:04 2024

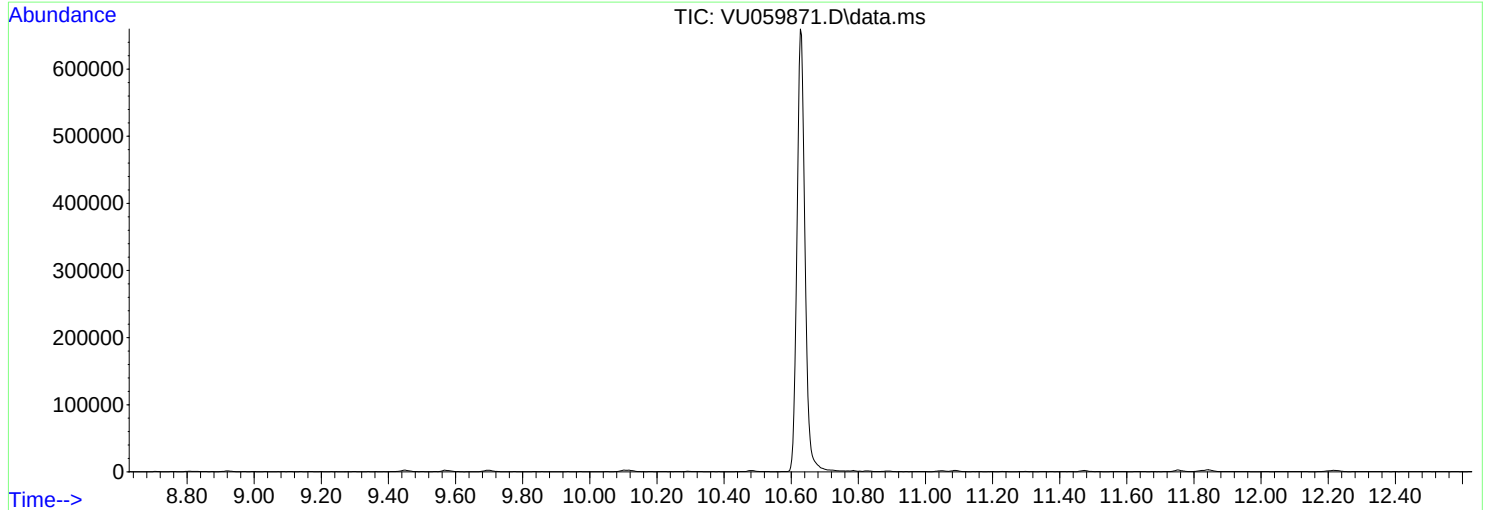

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	20563	PASS
75	95	30	80	48.6	61688	PASS
95	95	100	100	100.0	126851	PASS
96	95	5	9	6.8	8663	PASS
173	174	0.00	2	1.4	1592	PASS
174	95	50	120	90.0	114117	PASS
175	174	5	9	7.7	8799	PASS
176	174	95	101	96.8	110421	PASS
177	176	5	9	6.7	7398	PASS

Scan 2890 (10.582 min): VU059871.D\data.ms
BFB171

m/z	Abundance
39.80	140.0
43.90	351.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
35.90	881.0
36.90	4285.0
37.90	4152.0
38.90	1943.0
39.80	209.0
43.90	922.0
44.90	892.0
46.00	148.0
46.90	1140.0
47.80	511.0
49.00	4503.0
49.90	20080.0
50.90	6741.0
51.90	417.0
53.10	150.0
54.90	387.0
55.90	1670.0
57.00	3069.0
57.90	243.0
59.90	1041.0
61.00	6115.0
61.90	6087.0
62.90	5353.0
63.90	999.0
64.90	1178.0
65.90	166.0
66.90	311.0
67.90	11746.0
68.90	11841.0
69.90	956.0
71.00	116.0
71.90	548.0
72.90	5167.0
74.00	20136.0
75.00	58840.0
75.90	5678.0
76.90	791.0
77.90	567.0
78.80	5116.0
79.80	1251.0
80.90	4876.0
81.90	977.0
85.60	134.0
86.90	5578.0
87.90	5437.0
90.80	502.0
91.90	3418.0
92.90	5091.0
93.90	13484.0
95.00	120600.0
96.00	8362.0
97.00	206.0
103.80	540.0
104.80	190.0
105.80	502.0
106.80	126.0
107.80	116.0
114.80	190.0
115.80	465.0
116.90	1062.0
117.80	558.0
118.80	833.0
127.80	394.0
128.70	287.0
129.80	342.0
130.90	137.0
134.90	187.0
136.70	175.0
139.90	118.0
140.80	1094.0
141.70	168.0
142.90	1725.0
144.00	138.0
144.80	948.0
145.80	319.0
147.80	307.0
148.80	143.0
149.70	112.0
152.80	137.0
154.90	376.0
156.80	197.0
158.70	130.0
160.90	141.0
170.90	360.0
171.90	1622.0
172.90	1543.0
173.90	106016.0
174.90	8209.0
175.90	102744.0
176.90	7105.0
177.90	175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
35.90	902.0
36.90	4469.0
37.90	4219.0
38.90	2075.0
39.80	220.0
40.40	113.0
43.90	1033.0
44.90	903.0
46.00	177.0
46.90	1341.0
47.90	584.0
48.90	4981.0
49.90	21232.0
50.90	6941.0
51.90	396.0
53.00	125.0
53.80	131.0
54.80	372.0
55.90	1924.0
57.00	3361.0
57.90	194.0
59.90	1163.0
61.00	6448.0
61.90	6723.0
62.90	5891.0
63.90	997.0
64.90	1250.0
65.90	201.0
66.90	336.0
67.90	12544.0
68.90	12944.0
69.90	1055.0
71.90	637.0
72.90	5290.0
74.00	21880.0
75.00	63736.0
75.90	5907.0
76.90	918.0
77.90	622.0
78.80	5215.0
79.80	1307.0
80.90	5241.0
81.90	1010.0
85.60	104.0
86.90	6353.0
87.90	5781.0
90.80	539.0
91.90	3742.0
93.00	5633.0
93.90	14784.0
95.00	131040.0
96.00	8984.0
97.00	175.0
103.80	580.0
104.80	196.0
105.80	553.0
106.80	120.0
107.80	100.0
110.50	115.0
114.80	215.0
115.80	506.0
116.80	1004.0
117.80	473.0
118.80	968.0
127.80	455.0
128.70	269.0
129.80	446.0
130.90	150.0
134.90	173.0
136.70	165.0
139.90	121.0
140.80	1201.0
141.80	206.0
142.90	1982.0
143.90	111.0
144.80	1012.0
145.80	333.0
147.70	315.0
148.80	124.0
149.70	107.0
152.80	121.0
154.90	393.0
156.80	261.0
158.80	125.0
160.90	191.0
170.90	384.0
171.90	1790.0
172.90	1619.0
173.90	117640.0
174.90	9078.0
175.90	114096.0
176.90	7685.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

177.80

233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
35.90	834.0
36.90	4323.0
37.90	3897.0
38.90	2065.0
39.70	220.0
40.50	113.0
43.90	992.0
44.90	853.0
45.90	187.0
46.90	1356.0
47.90	671.0
48.90	4911.0
50.00	20376.0
50.90	6653.0
51.90	359.0
52.80	141.0
53.70	121.0
54.80	360.0
55.90	1912.0
57.00	3287.0
58.00	120.0
59.90	1193.0
60.90	6157.0
61.90	6507.0
62.90	5638.0
63.90	907.0
64.90	1191.0
65.90	205.0
66.90	326.0
67.90	12095.0
68.90	12565.0
69.90	1075.0
71.90	698.0
72.90	5080.0
74.00	21016.0
75.00	62488.0
75.90	5523.0
76.90	954.0
77.80	618.0
78.80	4795.0
79.80	1205.0
80.90	5085.0
81.90	993.0
85.50	100.0
86.10	129.0
86.90	6524.0
87.90	5470.0
90.80	500.0
91.90	3470.0
93.00	5627.0
94.00	14636.0
95.00	128912.0
96.00	8643.0
97.00	159.0
103.90	593.0
104.70	188.0
105.80	590.0
112.80	107.0
114.80	186.0
115.80	497.0
116.80	915.0
117.90	402.0
118.80	1035.0
127.90	425.0
128.80	203.0
129.80	496.0
130.90	145.0
134.90	156.0
136.70	123.0
140.90	1329.0
141.80	208.0
142.90	2118.0
144.80	999.0
145.80	287.0
147.70	316.0
153.90	100.0
154.80	388.0
156.90	285.0
158.80	142.0
160.80	197.0
170.90	425.0
171.90	1843.0
172.90	1613.0
173.90	118696.0
174.90	9111.0
175.90	114424.0
176.90	7404.0
177.80	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171