


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070918\
Data File : VU025263.D
Acq On : 09 Jul 2018 09:16
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U070918W.M
Title : SW846 8260
Last Update : Tue Jul 10 09:34:16 2018

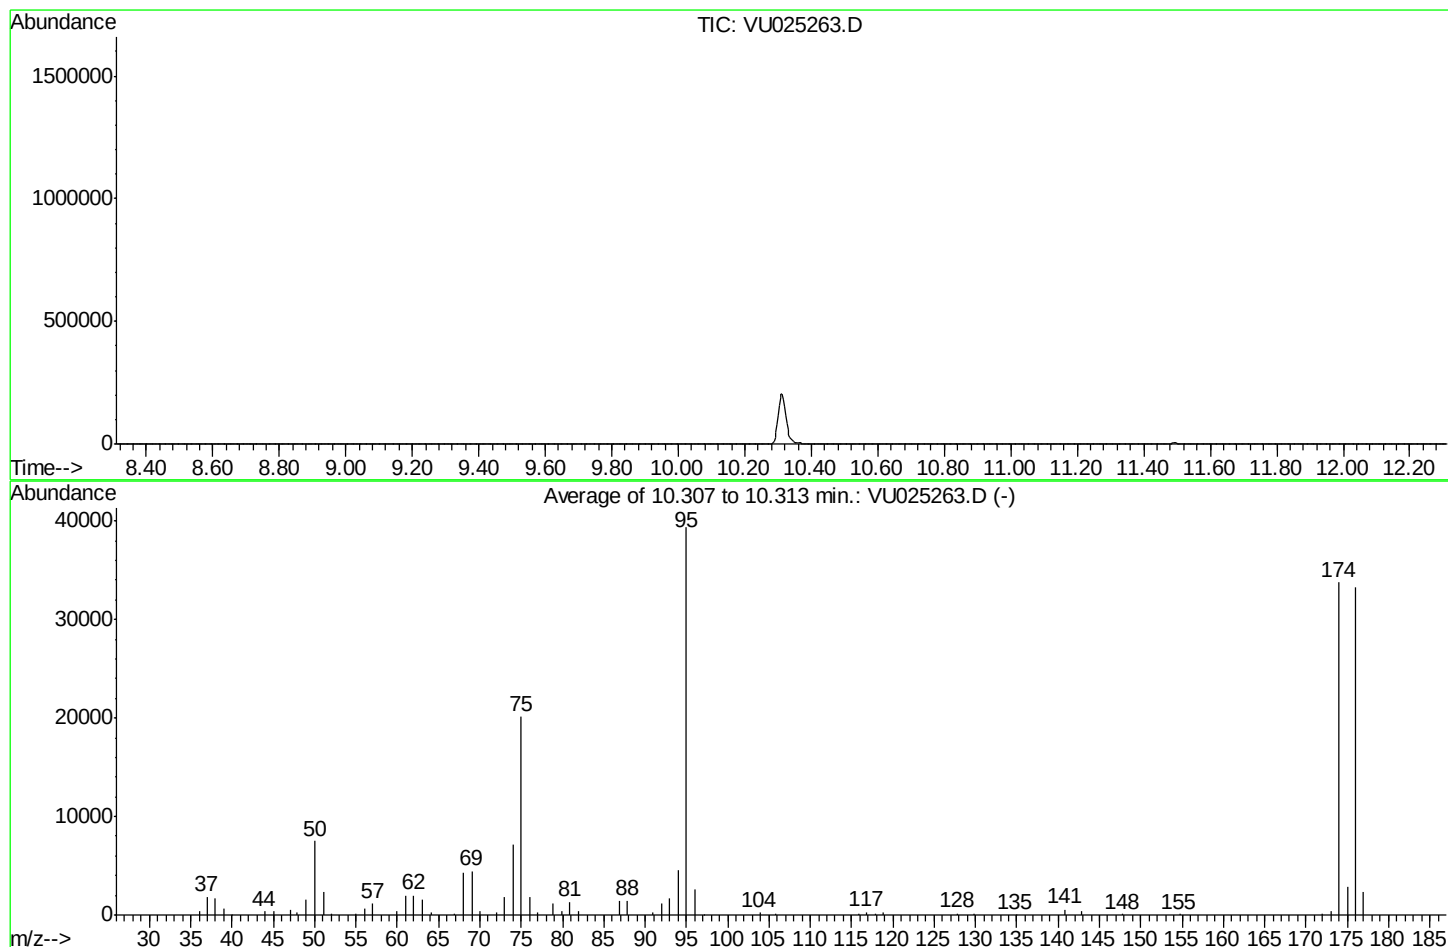

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	7538	PASS
75	95	30	60	51.1	20106	PASS
95	95	100	100	100.0	39370	PASS
96	95	5	9	6.7	2628	PASS
173	174	0.00	2	1.3	439	PASS
174	95	50	100	85.8	33784	PASS
175	174	5	9	8.4	2842	PASS
176	174	95	101	98.5	33288	PASS
177	176	5	9	6.9	2283	PASS