

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070920\
 Data File : VU039390.D
 Acq On : 09 Jul 2020 12:24
 Operator : SY/MD
 Sample : L3244-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4B14

Manual Integrations
 APPROVED

MMDadoda
 7/13/2020 10:49:58 AM

Quant Time: Jul 10 00:20:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 10 00:19:08 2020
 Response via : Initial Calibration

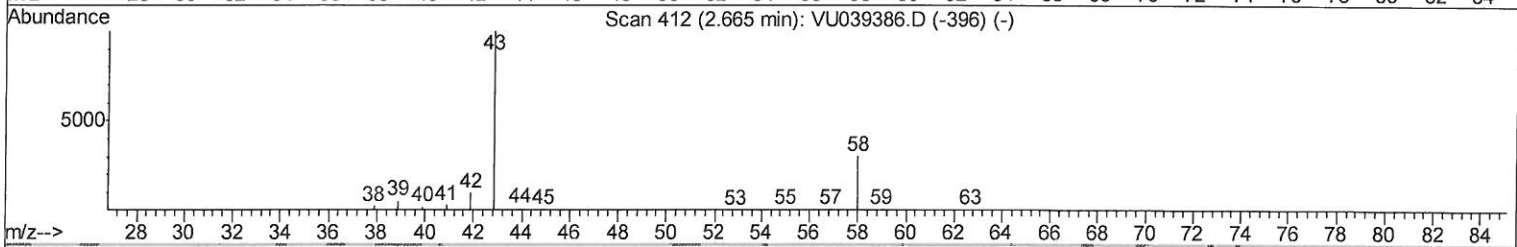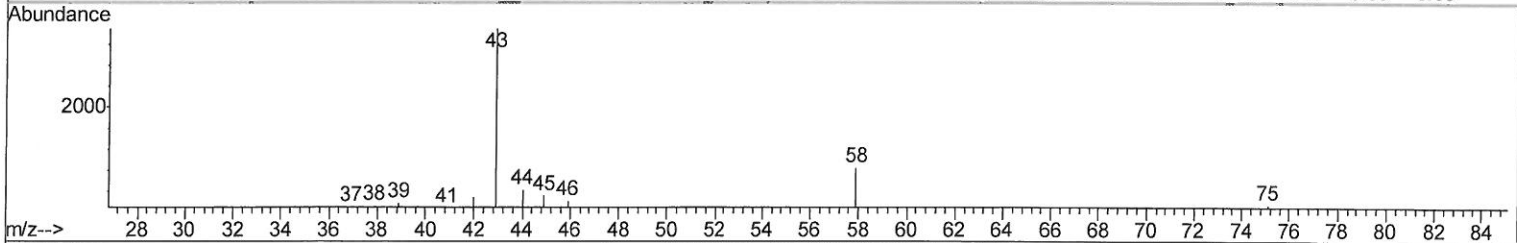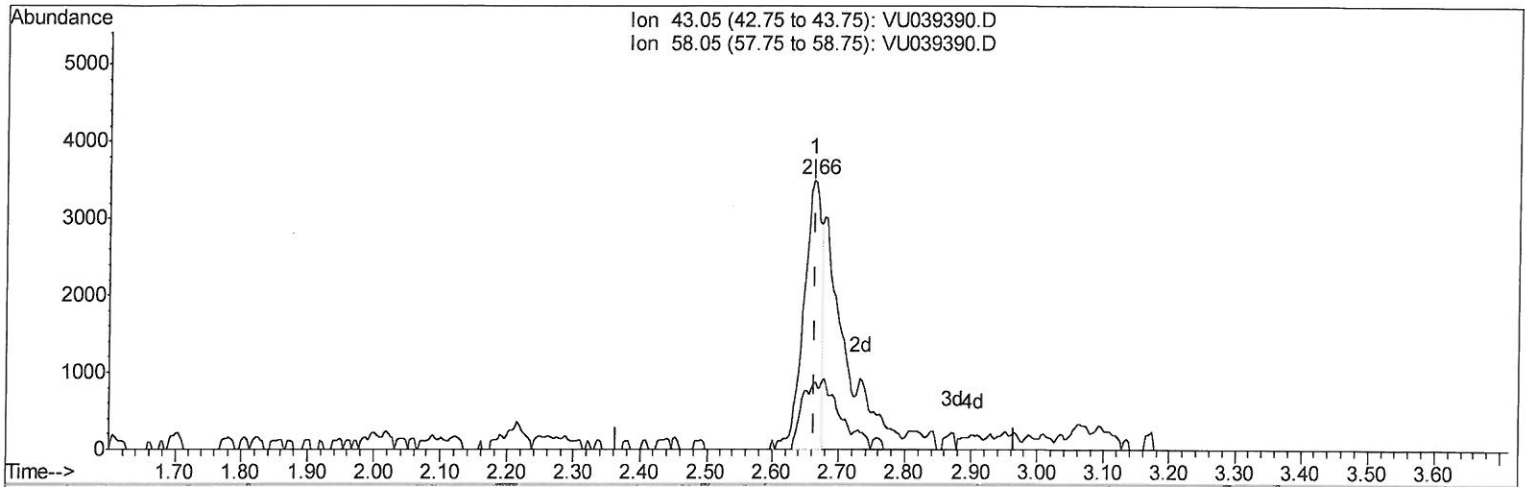

TIC: VU039390.D

(13) Acetone (T)

2.662min (-0.003) 4.57ug/L

response 6509

Ion	Exp%	Act%
43.05	100	100
58.05	31.40	21.98
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070920\
 Data File : VU039390.D
 Acq On : 09 Jul 2020 12:24
 Operator : SY/MD
 Sample : L3244-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4B14

Manual Integrations
 APPROVED

MMDadoda
 7/13/2020 10:49:58 AM

Quant Time: Jul 10 00:20:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 10 00:19:08 2020
 Response via : Initial Calibration

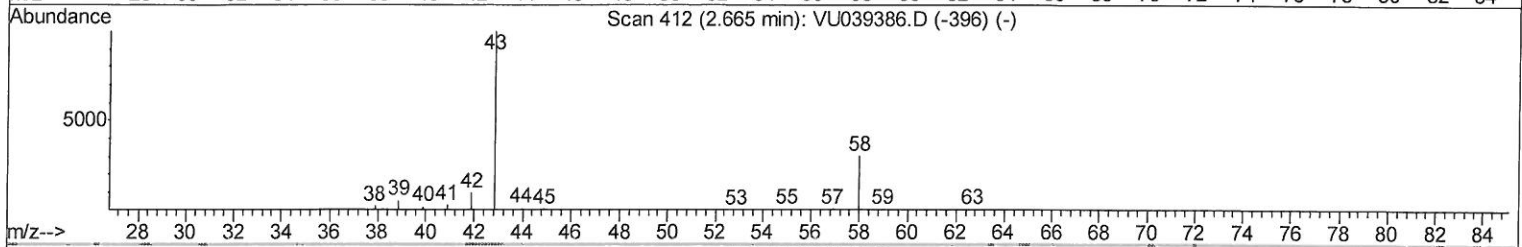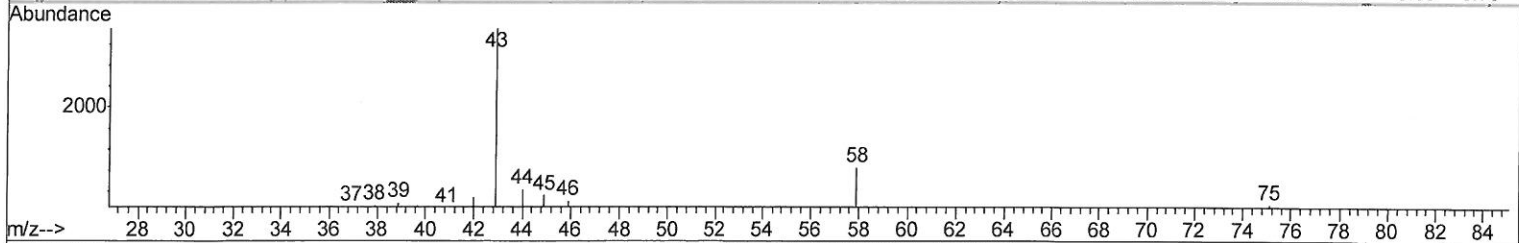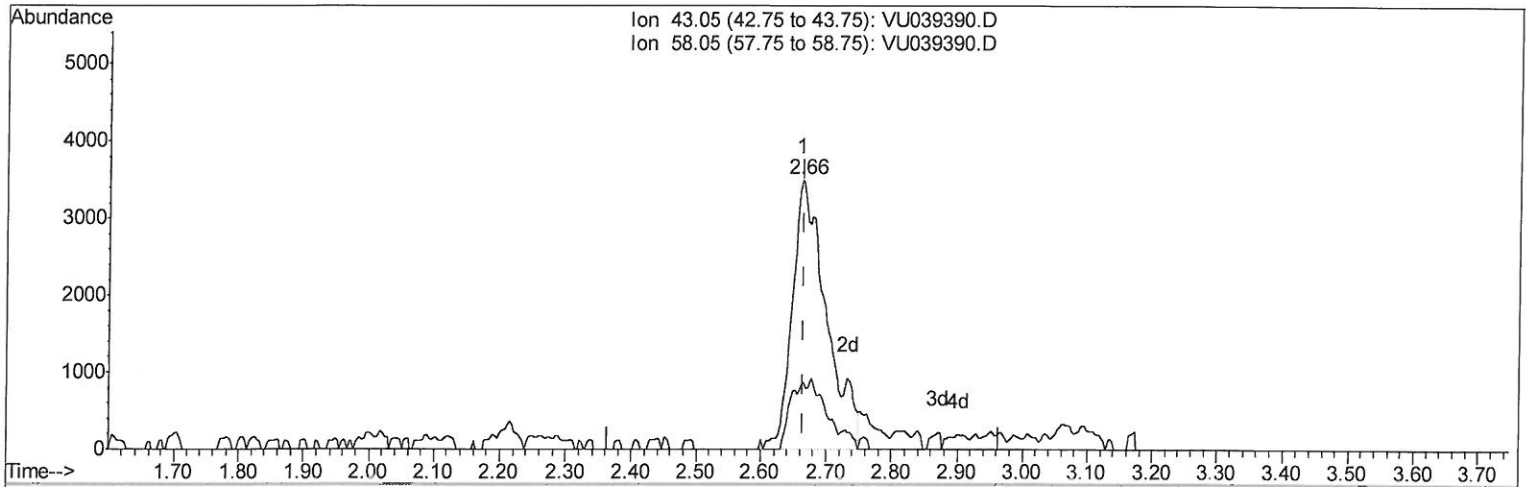

TIC: VU039390.D

(13) Acetone (T)

2.662min (-0.003) 8.91ug/L m

207114/2054

response 12680

Ion	Exp%	Act%
43.05	100	100
58.05	31.40	11.29
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070920\
 Data File : VU039390.D
 Acq On : 09 Jul 2020 12:24
 Operator : SY/MD
 Sample : L3244-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4B14

Manual Integrations
 APPROVED

MMDadoda
 7/13/2020 10:49:58 AM

Quant Time: Jul 10 00:38:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 10 00:19:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	99408	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	92620	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	44915	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.61	65	29195	5.07	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 101.40%			
7) Chloroethane-d5	1.93	69	29570	5.02	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 100.40%			
11) 1,1-Dichloroethene-d2	2.58	63	45475	4.01	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 80.20%			
20) 2-Butanone-d5	4.66	46	149019	56.53	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 113.06%			
24) Chloroform-d	5.08	84	66830	5.45	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 109.00%			
26) 1,2-Dichloroethane-d4	5.72	65	43950	5.71	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 114.20%			
32) Benzene-d6	5.75	84	129720	5.82	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 116.40%			
36) 1,2-Dichloropropane-d6	6.70	67	45652	5.83	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 116.60%			
41) Toluene-d8	7.91	98	112587	5.82	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 116.40%			
43) trans-1,3-Dichloropropene-	8.19	79	17610	5.09	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 101.80%			
46) 2-Hexanone-d5	8.64	63	110352	53.78	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 107.56%			
57) 1,1,2,2-Tetrachloroethane-	10.76	84	41484	5.34	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 106.80%			
64) 1,2-Dichlorobenzene-d4	12.19	152	46047	5.74	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 114.80%			
Target Compounds						
13) Acetone	2.66	43	12680m	8.911	ug/L	Ovalue
19) 1,1-Dichloroethane	3.89	63	2582	0.202	ug/L	99
22) cis-1,2-Dichloroethene	4.69	96	1270	0.173	ug/L	95
30) Cyclohexane	5.41	56	3132	0.273	ug/L	95
33) Benzene	5.79	78	3253	0.117	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU070920\
Data File : VU039390.D
Acq On : 09 Jul 2020 12:24
Operator : SY/MD
Sample : L3244-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4B14

Manual Integrations
APPROVED

MMDadoda
7/13/2020 10:49:58 AM

Quant Time: Jul 10 00:38:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 10 00:19:08 2020
Response via : Initial Calibration

