


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU070920\
 Data File : VU039385.D
 Acq On : 09 Jul 2020 08:54
 Operator : SY/MD
 Sample : BFB28
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB28

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jul 10 02:02:00 2020

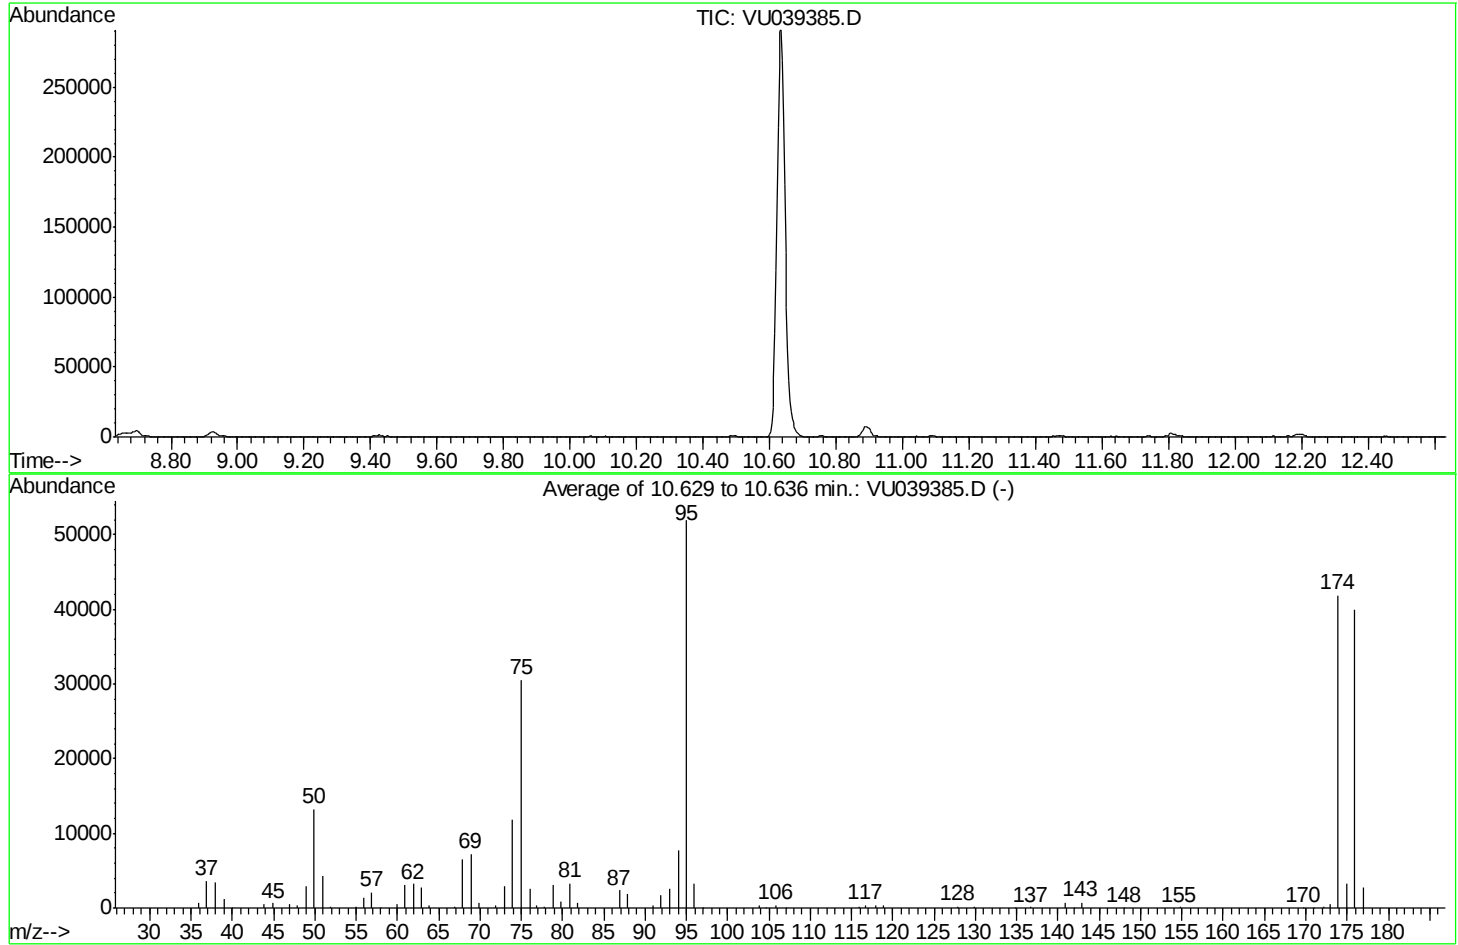

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.4	13210	PASS
75	95	30	80	58.8	30546	PASS
95	95	100	100	100.0	51938	PASS
96	95	5	9	6.2	3236	PASS
173	174	0.00	2	1.2	523	PASS
174	95	50	120	80.6	41845	PASS
175	174	5	9	7.7	3222	PASS
176	174	95	101	95.6	40016	PASS
177	176	5	9	6.7	2665	PASS

m/z	Abundance
35.90	602.0
36.90	3487.0
37.90	3337.0
38.90	1276.0
43.90	790.0
44.90	691.0
47.10	492.0
47.80	354.0
48.90	2767.0
49.90	12545.0
51.00	4162.0
51.90	177.0
55.00	209.0
55.90	1166.0
56.90	1995.0
60.00	514.0
60.90	2935.0
61.90	3177.0
62.90	2605.0
63.80	272.0
66.90	168.0
67.90	6243.0
68.90	6858.0
69.90	569.0
71.90	309.0
73.00	2815.0
73.90	10887.0
75.00	29256.0
76.00	2405.0
76.90	338.0
77.80	201.0
78.80	2834.0
79.80	871.0
80.90	3187.0
81.80	771.0
86.90	2130.0
87.90	1701.0
90.90	347.0
91.90	1633.0
92.90	2540.0
94.00	7207.0
95.00	49448.0
96.00	3180.0
96.90	125.0
103.70	309.0
105.90	360.0
115.90	239.0
116.70	341.0
117.90	307.0
118.80	322.0
127.80	183.0
129.90	175.0
136.70	110.0
140.90	665.0
142.80	681.0
148.00	117.0
154.80	139.0
172.20	216.0
172.90	458.0
173.90	39064.0
174.90	3121.0
175.90	35864.0
176.90	2559.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
35.90	641.0
36.90	3804.0
37.90	3588.0
39.00	1306.0
40.00	102.0
43.90	849.0
44.90	680.0
47.00	573.0
47.80	426.0
48.90	3074.0
49.90	13616.0
51.00	4393.0
51.90	168.0
54.90	240.0
55.90	1331.0
56.90	2170.0
57.90	126.0
60.00	619.0
60.90	3071.0
61.90	3323.0
63.00	2810.0
63.90	286.0
66.90	199.0
67.90	6679.0
68.90	7498.0
69.90	651.0
71.80	361.0
73.00	3019.0
73.90	12159.0
75.00	31416.0
76.00	2571.0
76.80	336.0
77.80	216.0
78.80	3125.0
79.90	922.0
80.90	3370.0
81.80	764.0
86.90	2472.0
87.90	2000.0
90.90	333.0
91.90	1800.0
93.00	2699.0
94.00	8040.0
95.00	53392.0
95.90	3282.0
97.00	144.0
103.80	284.0
105.90	374.0
107.00	101.0
115.80	250.0
116.70	375.0
117.90	301.0
118.90	330.0
127.80	222.0
129.80	193.0
134.80	106.0
136.70	142.0
140.90	746.0
141.90	103.0
142.80	794.0
148.00	111.0
154.80	164.0
169.70	102.0
172.20	201.0
172.90	489.0
173.90	43088.0
174.90	3345.0
175.90	41240.0
176.90	2714.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
35.90	608.0
36.90	3589.0
37.90	3520.0
39.00	1241.0
43.90	868.0
45.00	583.0
46.90	671.0
47.80	440.0
49.00	3125.0
49.90	13469.0
51.00	4193.0
51.90	170.0
54.90	246.0
55.90	1390.0
56.90	2250.0
57.90	148.0
60.00	636.0
61.00	3211.0
61.90	3260.0
63.00	2771.0
63.90	283.0
66.90	158.0
67.90	6524.0
68.90	7478.0
69.90	690.0
71.80	384.0
72.90	3010.0
73.90	12291.0
75.00	30968.0
76.00	2582.0
76.80	343.0
77.70	213.0
78.80	3280.0
79.90	841.0
80.90	3292.0
81.80	685.0
86.90	2545.0
87.90	2152.0
90.90	350.0
91.90	1764.0
93.00	2658.0
94.00	8109.0
95.00	52976.0
95.90	3246.0
103.80	277.0
104.60	134.0
105.90	400.0
115.80	238.0
116.70	390.0
117.90	263.0
118.90	348.0
127.90	228.0
129.80	231.0
136.70	133.0
140.90	750.0
141.90	106.0
142.90	852.0
154.80	163.0
171.00	125.0
172.10	188.0
172.90	623.0
173.90	43384.0
174.90	3202.0
175.90	42944.0
176.90	2724.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
43.80	260.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28