


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071018\
Data File : VU025280.D
Acq On : 10 Jul 2018 09:46
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U070918W.M
Title : SW846 8260
Last Update : Tue Jul 10 09:34:16 2018

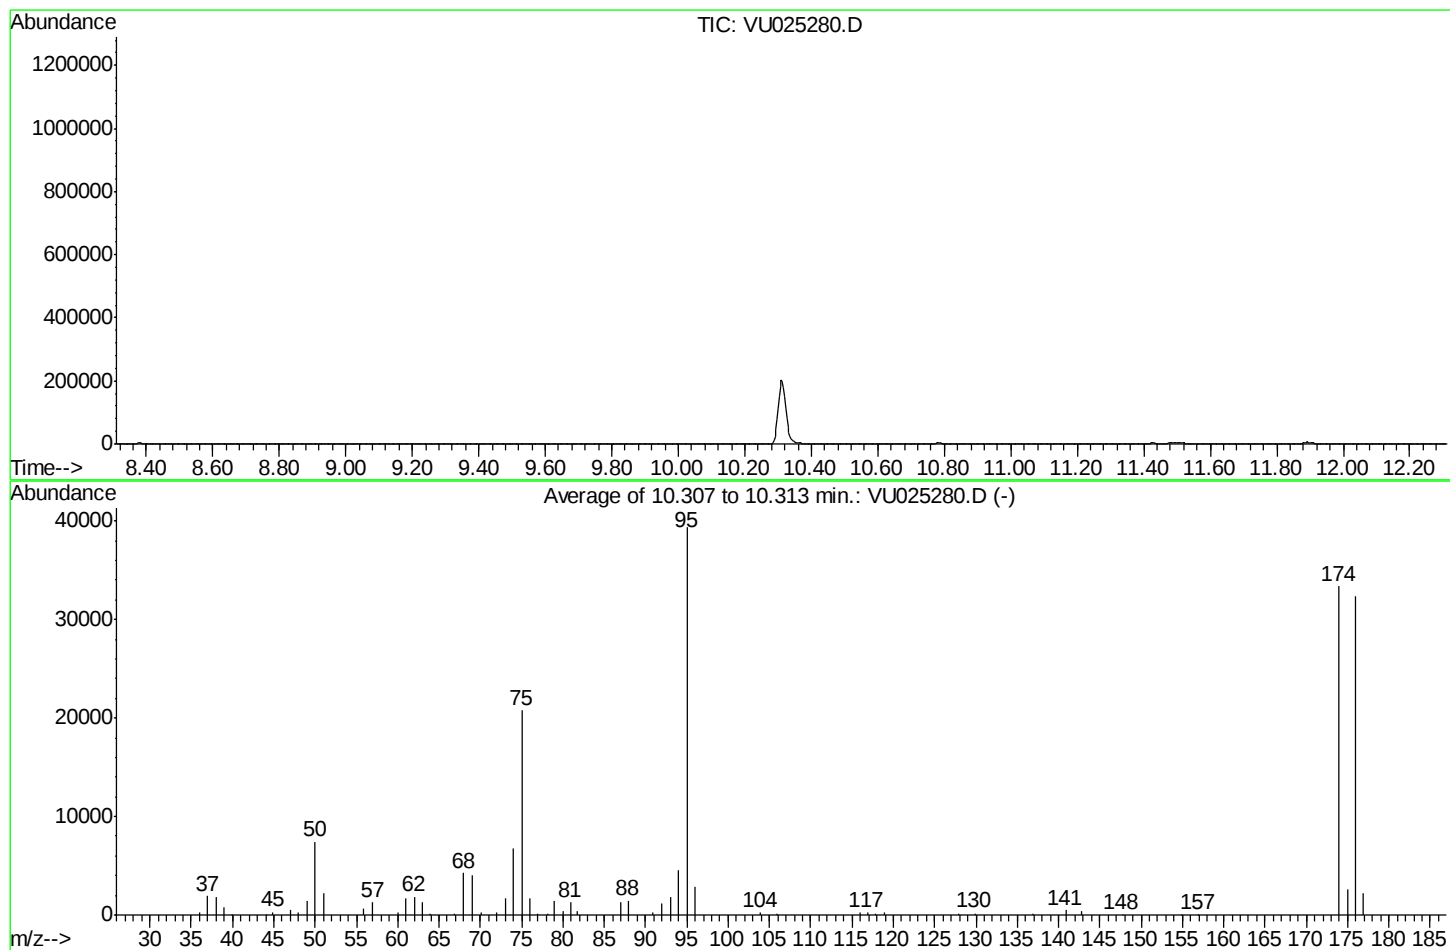

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	7414	PASS
75	95	30	60	52.8	20765	PASS
95	95	100	100	100.0	39352	PASS
96	95	5	9	7.3	2892	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.8	33370	PASS
175	174	5	9	7.6	2545	PASS
176	174	95	101	97.0	32370	PASS
177	176	5	9	7.0	2271	PASS