

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071020\
 Data File : VU039448.D
 Acq On : 10 Jul 2020 22:15
 Operator : SY/MD
 Sample : L3268-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A74

Quant Time: Jul 11 04:36:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 11 02:49:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	94027	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	86625	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	42748	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	19743	3.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.40%
7) Chloroethane-d5	1.93	69	25833	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.60%
11) 1,1-Dichloroethene-d2	2.58	63	33583	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	4.66	46	150012	60.16	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.32%
24) Chloroform-d	5.09	84	58087	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
26) 1,2-Dichloroethane-d4	5.72	65	38726	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.40%
32) Benzene-d6	5.75	84	107487	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
36) 1,2-Dichloropropane-d6	6.71	67	38966	5.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.40%
41) Toluene-d8	7.91	98	91932	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
43) trans-1,3-Dichloropropene-	8.19	79	14935	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.64	63	108535	56.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.10%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	37558	5.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	38504	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
13) Acetone	2.66	43	3859	2.867 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071020\
Data File : VU039448.D
Acq On : 10 Jul 2020 22:15
Operator : SY/MD
Sample : L3268-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A74

Quant Time: Jul 11 04:36:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 11 02:49:36 2020
Response via : Initial Calibration

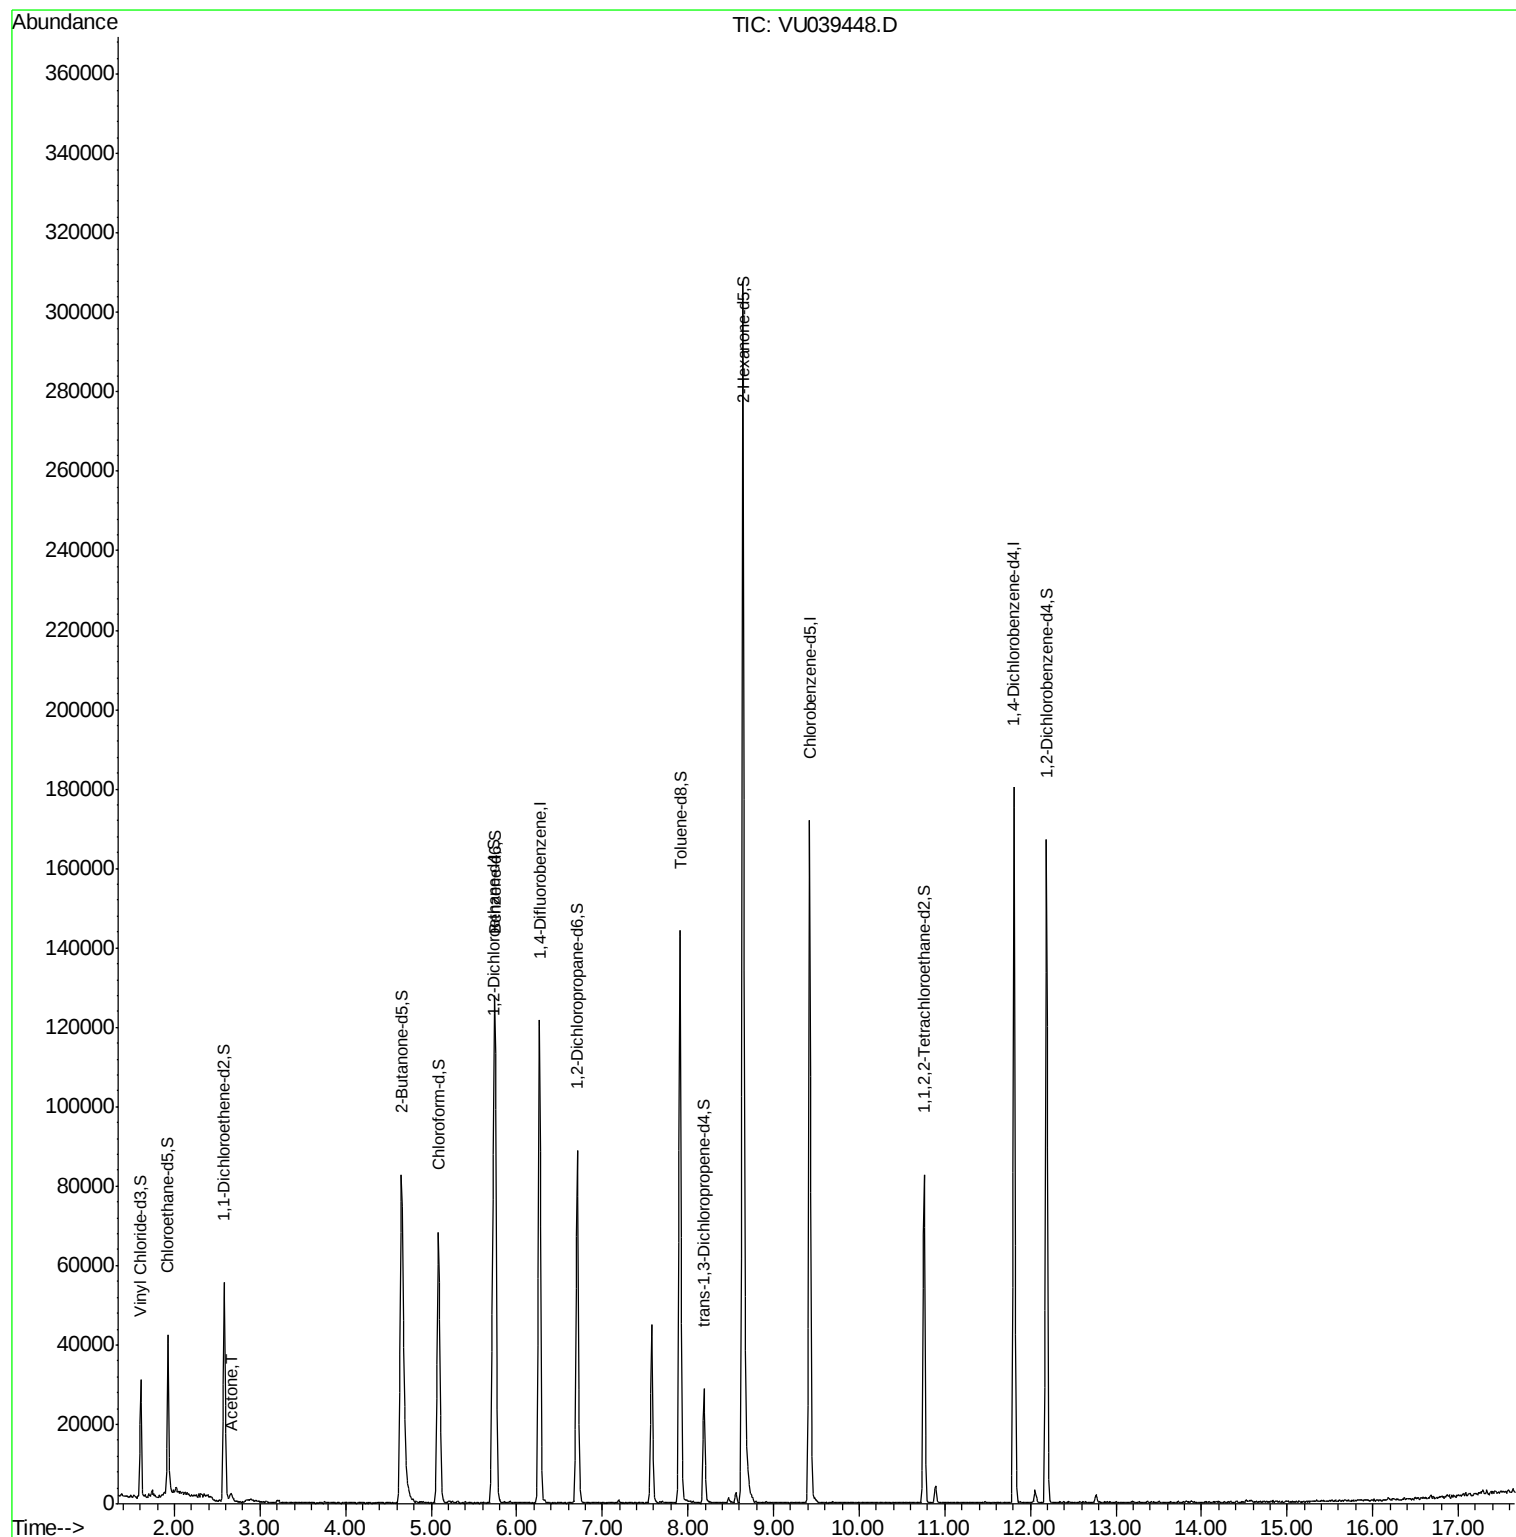

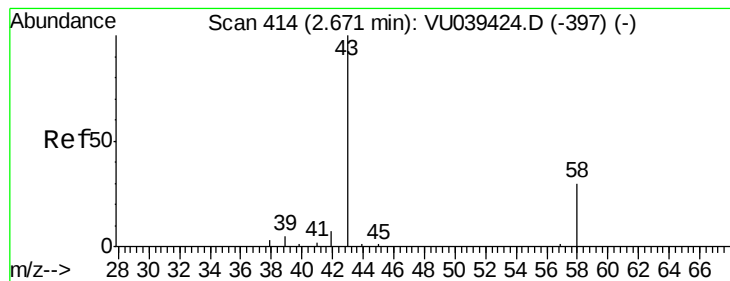

#13

Acetone

Concen: 2.867 ug/L

RT: 2.66 min Scan# 411

Delta R.T. -0.01 min

Lab File: VU039448.D

Acq: 10 Jul 2020 22:15

Instrument :
MSVOA_U
ClientSampleId :
F4A74

Tot Ion: 43 Resp: 3859

Ion Ratio Lower Upper

43 100

58 27.2 0.0 62.8

