


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071020\
 Data File : VU039423.D
 Acq On : 10 Jul 2020 11:56
 Operator : SY/MD
 Sample : BFB29
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB29

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jul 13 01:44:04 2020

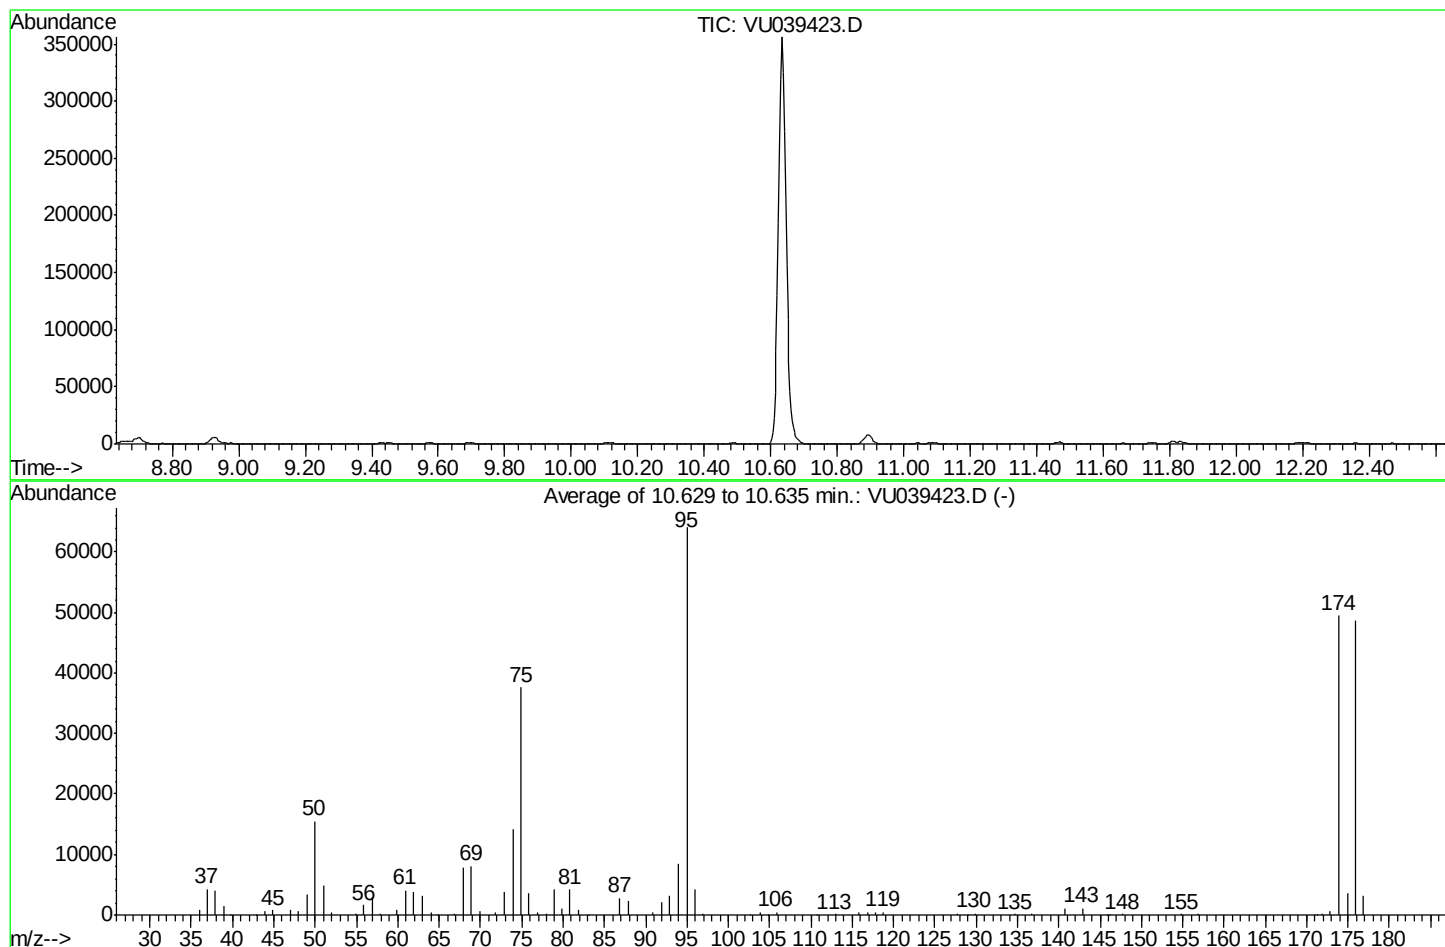

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	15464	PASS
75	95	30	80	58.8	37658	PASS
95	95	100	100	100.0	64074	PASS
96	95	5	9	6.7	4271	PASS
173	174	0.00	2	1.4	697	PASS
174	95	50	120	77.3	49504	PASS
175	174	5	9	7.1	3529	PASS
176	174	95	101	98.3	48674	PASS
177	176	5	9	6.4	3092	PASS

Scan 2876 (10.587 min): VU039423.D
BFB29

m/z	Abundance
39.70	120.0
43.90	359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.90	842.0
36.90	4024.0
37.90	3822.0
38.90	1566.0
39.90	173.0
42.80	111.0
43.90	848.0
44.90	809.0
47.00	759.0
47.90	543.0
49.00	3220.0
50.00	14181.0
51.00	4727.0
51.90	338.0
54.90	320.0
55.90	1485.0
56.90	2602.0
57.80	140.0
59.90	769.0
60.90	3827.0
62.00	3623.0
62.90	2990.0
64.00	452.0
66.80	222.0
67.90	7736.0
68.90	7518.0
69.90	665.0
71.90	376.0
73.00	3568.0
74.00	13556.0
75.00	34808.0
75.90	3467.0
76.80	335.0
78.00	307.0
78.90	3899.0
79.80	930.0
80.80	4001.0
81.90	695.0
86.90	2689.0
87.90	2344.0
90.80	434.0
91.90	1958.0
92.90	3194.0
93.90	7714.0
95.00	59824.0
96.00	4104.0
97.00	137.0
103.80	381.0
105.90	390.0
110.70	135.0
113.00	147.0
115.80	341.0
116.90	456.0
117.80	339.0
118.80	466.0
127.70	248.0
129.00	102.0
129.90	256.0
134.80	144.0
136.70	196.0
140.80	1117.0
142.90	1005.0
147.80	153.0
154.90	182.0
156.80	121.0
170.90	124.0
171.90	220.0
172.80	675.0
173.90	44928.0
174.90	3360.0
175.90	43968.0
176.90	2821.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.90	858.0
36.90	4422.0
37.90	4183.0
38.90	1590.0
39.80	154.0
42.80	103.0
43.90	919.0
44.90	888.0
47.00	955.0
47.90	555.0
49.00	3468.0
49.90	15967.0
51.00	5038.0
52.00	371.0
54.90	335.0
55.90	1720.0
56.90	3100.0
57.80	143.0
59.90	834.0
61.00	4143.0
61.90	3868.0
62.90	3194.0
64.00	434.0
64.90	114.0
66.90	274.0
67.90	8095.0
68.90	8334.0
69.90	676.0
71.80	438.0
73.00	3933.0
74.00	14702.0
74.90	39128.0
75.90	3623.0
76.90	372.0
78.00	324.0
78.90	4308.0
79.80	1095.0
80.90	4362.0
81.80	833.0
83.10	127.0
86.90	2894.0
87.90	2473.0
90.80	442.0
91.90	2130.0
92.90	3360.0
93.90	8679.0
95.00	66256.0
96.00	4400.0
97.00	150.0
103.80	453.0
104.90	115.0
105.80	488.0
110.70	137.0
113.00	188.0
115.80	384.0
116.90	500.0
117.80	395.0
118.80	537.0
127.70	309.0
129.00	104.0
129.80	321.0
134.80	164.0
136.70	171.0
140.80	1133.0
142.90	1139.0
146.10	120.0
147.80	116.0
154.90	187.0
156.80	186.0
171.00	129.0
171.90	239.0
172.90	718.0
173.90	51144.0
174.90	3579.0
175.90	50096.0
176.90	3219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
36.00	750.0
36.90	4368.0
37.90	4078.0
38.90	1440.0
39.80	123.0
44.00	1005.0
44.90	810.0
47.00	1018.0
47.90	531.0
48.90	3368.0
49.90	16246.0
51.00	4889.0
52.00	326.0
54.90	288.0
55.90	1720.0
56.90	3121.0
57.80	117.0
59.90	758.0
60.90	4144.0
61.90	3742.0
62.90	3134.0
64.00	343.0
64.90	114.0
66.90	283.0
67.90	7826.0
68.90	8296.0
69.90	750.0
71.80	423.0
72.90	3777.0
73.90	14545.0
74.90	39040.0
75.90	3457.0
77.00	438.0
78.00	287.0
78.80	4384.0
79.80	1134.0
80.90	4283.0
81.80	945.0
83.10	144.0
86.90	2847.0
87.90	2327.0
90.80	427.0
91.90	2150.0
92.90	3232.0
93.90	8886.0
95.00	66144.0
96.00	4310.0
96.90	149.0
102.70	117.0
103.80	480.0
104.80	147.0
105.80	525.0
113.00	156.0
115.90	372.0
116.90	522.0
117.80	373.0
118.80	514.0
127.80	301.0
129.80	345.0
134.70	176.0
136.60	114.0
140.80	948.0
142.90	1136.0
145.80	116.0
147.70	126.0
154.90	196.0
156.80	170.0
171.30	128.0
171.90	229.0
172.90	698.0
173.90	52440.0
174.90	3648.0
175.90	51960.0
176.90	3236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29