


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071024\
Data File : VU059889.D
Acq On : 10 Jul 2024 07:58
Operator : MD/SY
Sample : BFB172
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB172

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jul 11 01:53:22 2024

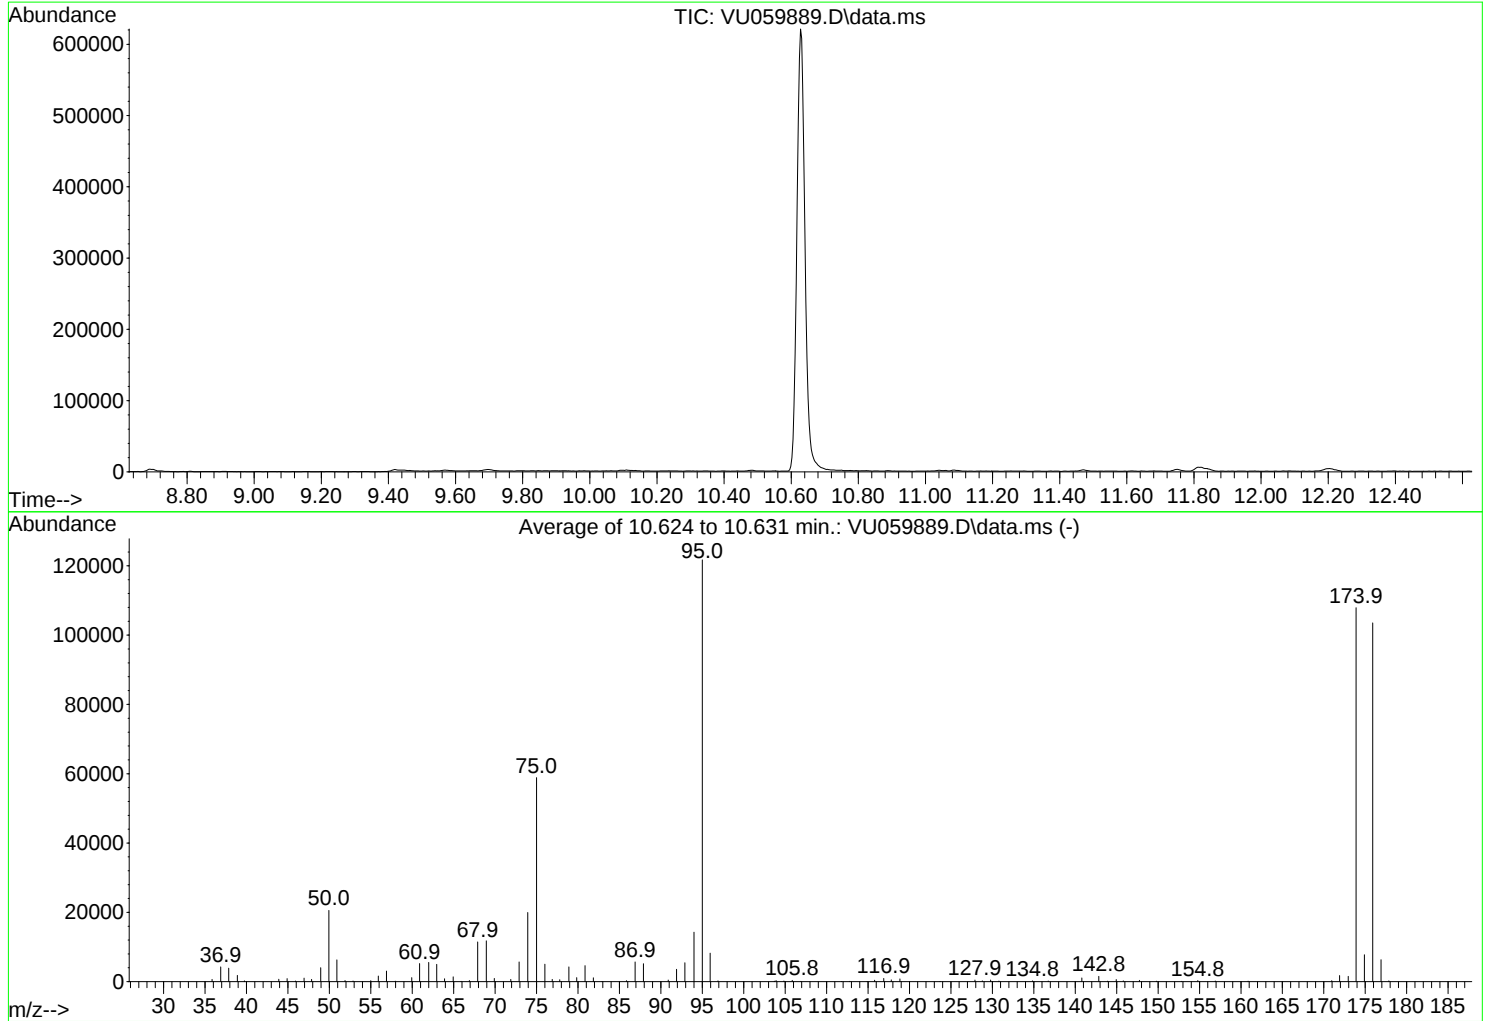

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	20560	PASS
75	95	30	80	48.4	58893	PASS
95	95	100	100	100.0	121728	PASS
96	95	5	9	6.7	8216	PASS
173	174	0.00	2	1.4	1525	PASS
174	95	50	120	88.6	107901	PASS
175	174	5	9	7.2	7781	PASS
176	174	95	101	95.9	103523	PASS
177	176	5	9	6.1	6331	PASS

m/z	Abundance
35.90	666.0
37.90	292.0
44.00	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
35.90	1139.0
36.90	4059.0
37.90	4043.0
38.90	1771.0
39.80	224.0
43.90	798.0
44.90	895.0
45.90	173.0
46.90	917.0
47.90	623.0
48.90	3996.0
49.90	20568.0
50.90	6016.0
51.90	298.0
52.80	211.0
55.00	286.0
55.90	1766.0
56.90	2921.0
57.90	116.0
60.00	1100.0
60.90	5183.0
62.00	5483.0
62.90	4864.0
63.90	866.0
64.90	1496.0
65.90	140.0
67.00	352.0
67.90	11243.0
68.90	11684.0
69.90	903.0
71.90	655.0
72.90	5326.0
74.00	19176.0
75.00	57256.0
76.00	4973.0
76.80	565.0
77.80	654.0
78.90	4226.0
79.80	1122.0
80.90	4433.0
81.90	1063.0
82.90	149.0
85.90	304.0
86.90	5580.0
87.90	4967.0
90.90	469.0
91.90	3372.0
92.90	5188.0
94.00	13769.0
95.00	118896.0
96.00	7903.0
96.90	208.0
103.70	421.0
104.80	183.0
105.80	378.0
114.90	107.0
115.80	380.0
116.90	885.0
117.80	521.0
118.80	681.0
127.90	411.0
128.80	188.0
129.70	400.0
130.80	180.0
134.90	199.0
136.70	148.0
140.80	1049.0
142.80	1600.0
143.80	163.0
145.00	594.0
145.80	195.0
147.70	323.0
149.80	120.0
154.80	237.0
156.90	172.0
160.80	141.0
170.90	233.0
171.90	1687.0
172.90	1485.0
173.90	102168.0
174.90	7420.0
175.90	97000.0
176.90	6002.0
177.80	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
35.90	1319.0
36.90	4369.0
37.90	4280.0
38.90	1839.0
39.70	248.0
43.90	973.0
44.90	887.0
45.90	210.0
46.90	1042.0
47.80	664.0
49.00	4128.0
49.90	21304.0
50.90	6499.0
51.90	349.0
52.80	211.0
55.00	273.0
55.90	1687.0
56.90	3176.0
57.90	161.0
59.90	1226.0
60.90	5374.0
62.00	5697.0
63.00	5218.0
63.90	893.0
65.00	1384.0
65.90	124.0
66.90	354.0
67.90	11847.0
69.00	12138.0
69.90	977.0
71.90	676.0
72.90	5897.0
73.90	20520.0
75.00	60544.0
76.00	5189.0
76.90	648.0
77.80	601.0
78.90	4261.0
79.90	1175.0
80.80	4760.0
81.80	1149.0
85.80	302.0
86.90	5900.0
87.90	5325.0
90.90	471.0
91.90	3660.0
92.90	5586.0
94.00	14631.0
95.00	125320.0
96.00	8521.0
96.90	254.0
103.90	443.0
104.90	169.0
105.80	381.0
106.90	102.0
111.80	103.0
112.80	106.0
115.80	444.0
116.90	964.0
117.80	561.0
118.90	796.0
127.90	476.0
128.80	236.0
129.80	482.0
130.80	177.0
134.80	223.0
136.70	180.0
140.80	1123.0
142.80	1577.0
143.90	158.0
145.00	628.0
145.80	238.0
147.80	366.0
149.80	138.0
152.80	119.0
154.80	343.0
156.90	200.0
160.80	139.0
170.90	262.0
171.90	1758.0
172.90	1550.0
173.90	111296.0
174.90	7987.0
175.90	106648.0
176.90	6514.0
177.90	266.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
35.90	1456.0
36.90	4383.0
37.90	4225.0
38.90	1804.0
39.70	186.0
43.90	1026.0
44.90	833.0
45.90	209.0
47.00	1138.0
47.90	671.0
48.90	3879.0
50.00	19808.0
50.90	6304.0
51.90	392.0
52.90	188.0
55.00	267.0
55.90	1448.0
56.90	3057.0
58.00	162.0
59.90	1146.0
60.90	5081.0
62.00	5460.0
63.00	4947.0
63.90	801.0
65.00	1214.0
66.80	303.0
67.90	11211.0
69.00	11522.0
69.90	914.0
71.90	644.0
72.90	5863.0
73.90	20096.0
75.00	58880.0
76.00	5007.0
77.00	735.0
77.80	449.0
78.90	4216.0
79.90	1176.0
80.80	4681.0
81.80	1115.0
85.80	263.0
86.90	5614.0
87.90	5305.0
90.90	406.0
91.90	3660.0
92.90	5611.0
94.00	14420.0
95.00	120968.0
95.90	8225.0
96.90	282.0
103.90	513.0
104.90	174.0
105.80	413.0
106.90	114.0
111.80	101.0
112.80	118.0
115.80	475.0
116.90	939.0
117.80	517.0
118.90	816.0
123.70	100.0
127.90	472.0
128.80	256.0
129.90	475.0
130.80	174.0
134.80	260.0
136.80	213.0
140.80	1072.0
142.90	1434.0
144.00	133.0
144.90	599.0
145.80	243.0
147.70	372.0
149.80	160.0
152.80	150.0
154.80	376.0
156.90	187.0
160.90	100.0
171.00	291.0
171.90	1764.0
173.00	1540.0
173.90	110240.0
174.90	7937.0
175.90	106920.0
176.90	6476.0
177.90	290.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172