


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071025\
Data File : VU063467.D
Acq On : 10 Jul 2025 08:28
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U070825W.M
Title : SW846 8260
Last Update : Wed Jul 09 04:25:34 2025

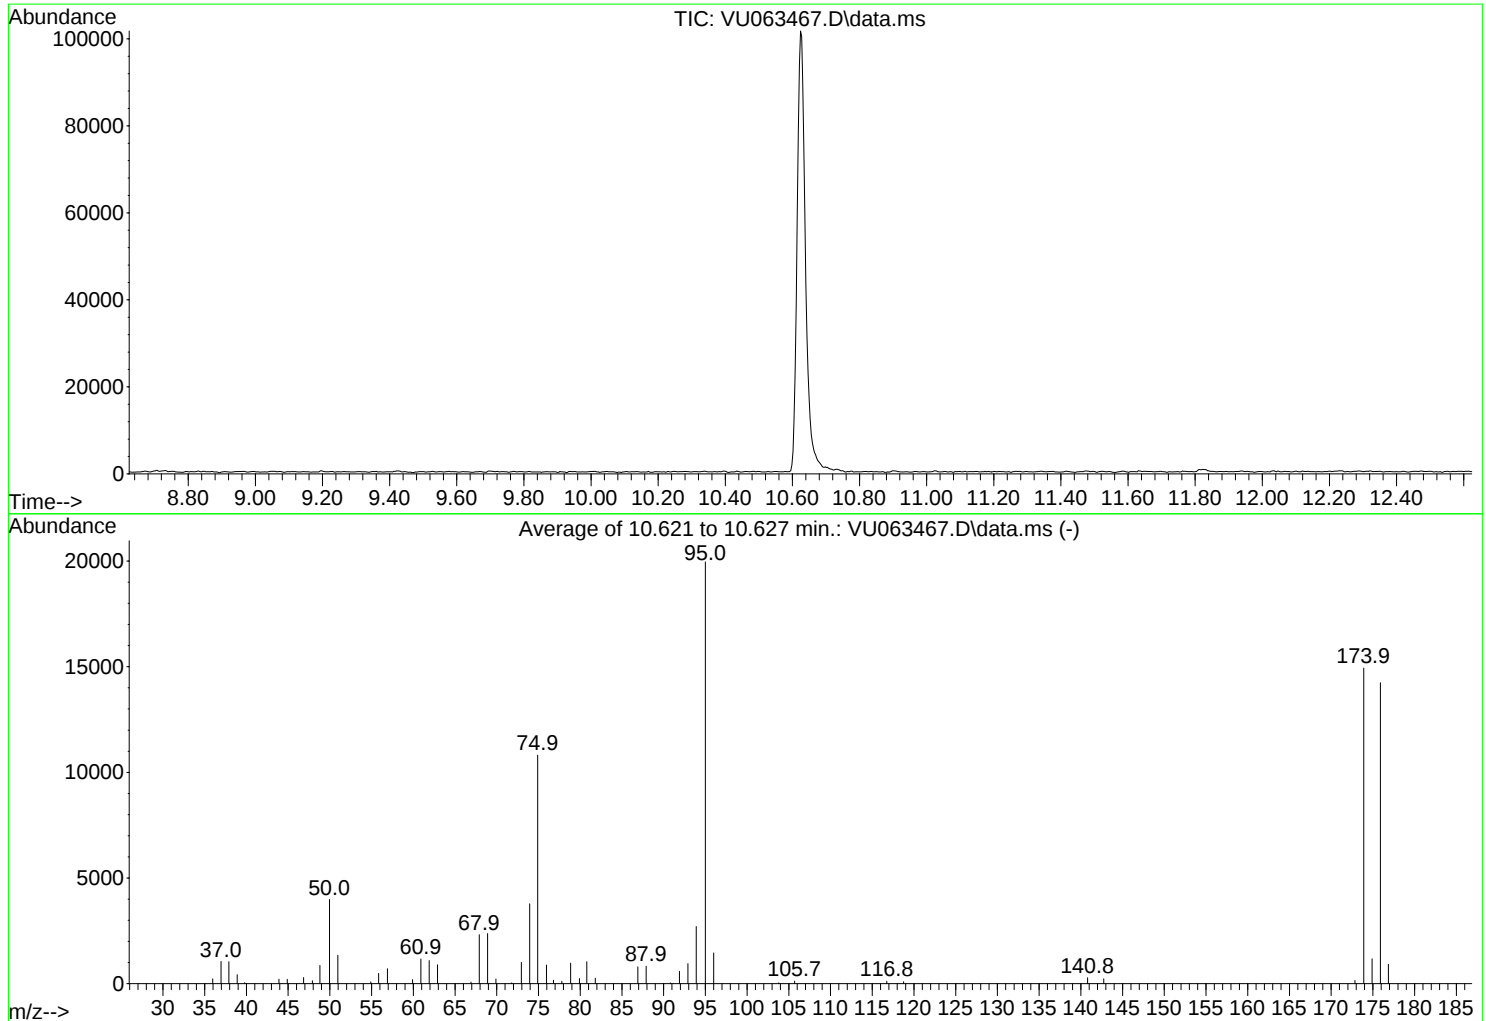

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	3983	PASS
75	95	30	60	54.2	10818	PASS
95	95	100	100	100.0	19965	PASS
96	95	5	9	7.3	1455	PASS
173	174	0.00	2	1.0	155	PASS
174	95	50	100	74.8	14935	PASS
175	174	5	9	7.8	1171	PASS
176	174	95	101	95.4	14242	PASS
177	176	5	9	6.4	916	PASS