


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071118\
Data File : VU025305.D
Acq On : 11 Jul 2018 09:38
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U070918W.M
Title : SW846 8260
Last Update : Tue Jul 10 09:34:16 2018

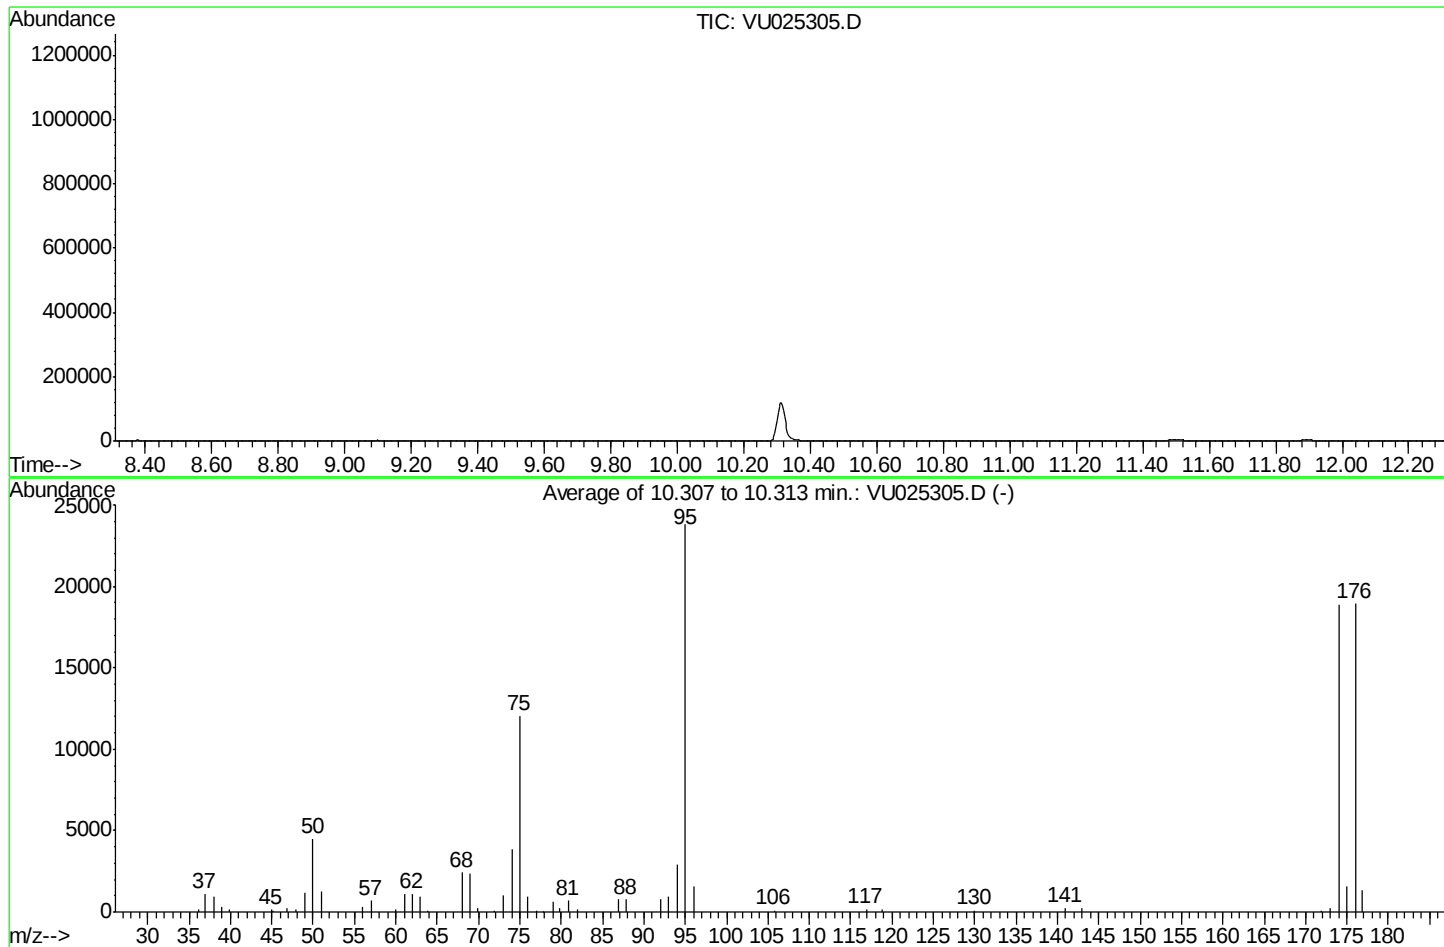

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	4483	PASS
75	95	30	60	50.7	12074	PASS
95	95	100	100	100.0	23818	PASS
96	95	5	9	6.7	1590	PASS
173	174	0.00	2	1.2	219	PASS
174	95	50	100	79.2	18866	PASS
175	174	5	9	8.3	1558	PASS
176	174	95	101	100.4	18946	PASS
177	176	5	9	7.3	1377	PASS